
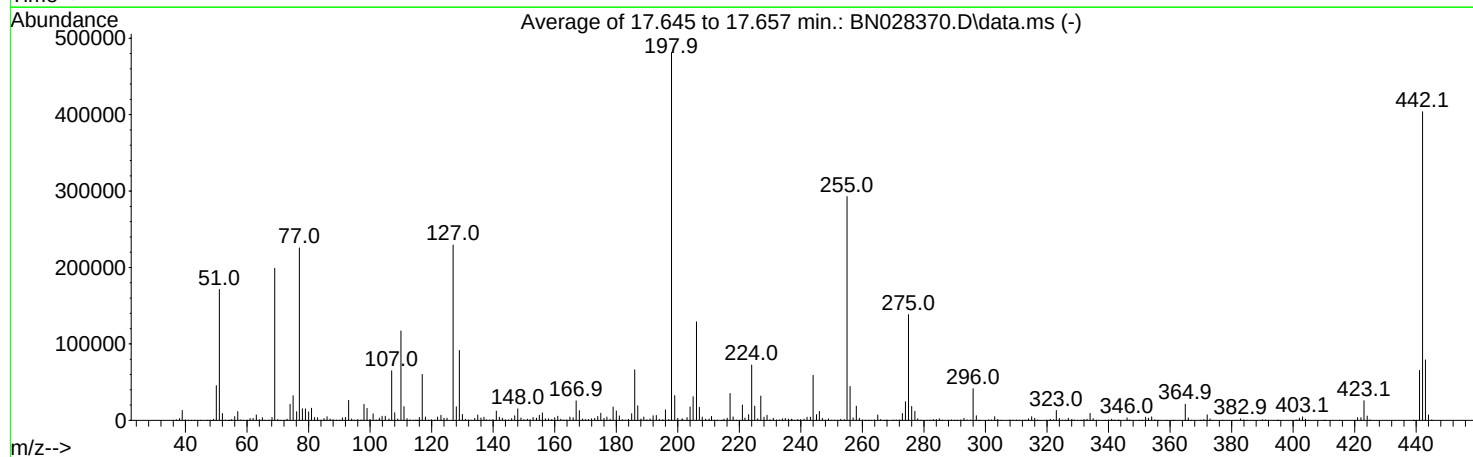


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102423\
 Data File : BN028370.D
 Acq On : 24 Oct 2023 10:09
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN101223.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 23 15:14:08 2023

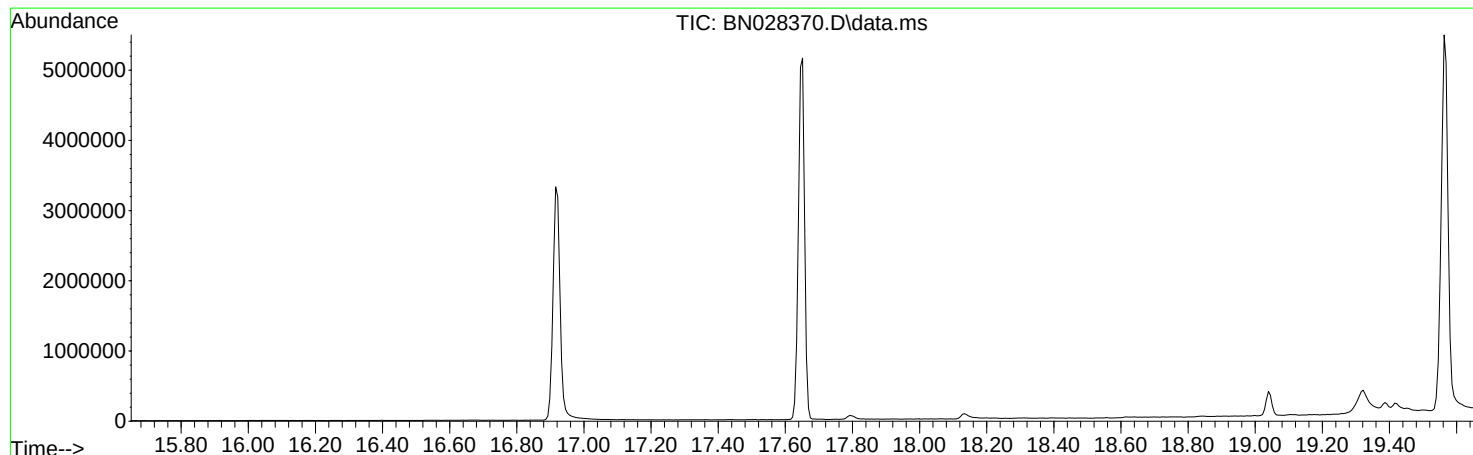




AutoFind: Scans 2509, 2510, 2511; Background Corrected with Scan 2501

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.6	171235	PASS
68	69	0.00	2	1.9	3706	PASS
69	198	0.00	100	41.4	199203	PASS
70	69	0.00	2	0.5	997	PASS
127	198	10	80	47.7	229376	PASS
197	198	0.00	2	0.3	1357	PASS
198	198	100	100	100.0	481323	PASS
199	198	5	9	6.8	32563	PASS
275	198	10	60	28.7	138296	PASS
365	198	1	100	4.4	21259	PASS
441	198	0.01	100	13.6	65352	PASS
442	442	50	100	100.0	403840	PASS
443	442	15	24	19.6	79208	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102423\
Data File : BN028370.D
Acq On : 24 Oct 2023 10:09
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 25 05:13:45 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 25 05:13:40 2023
Response via : Initial Calibration

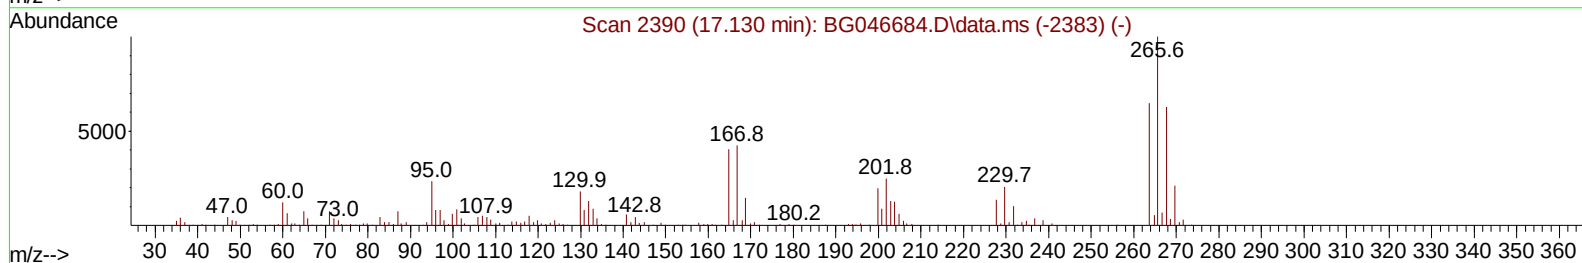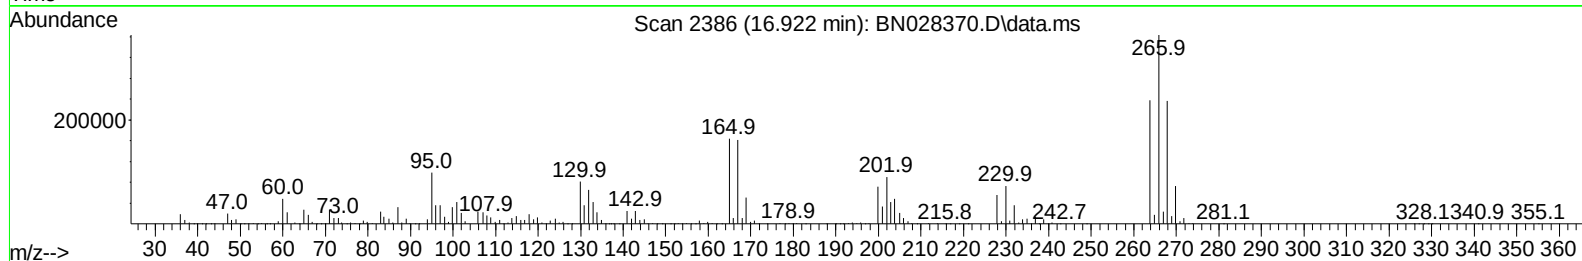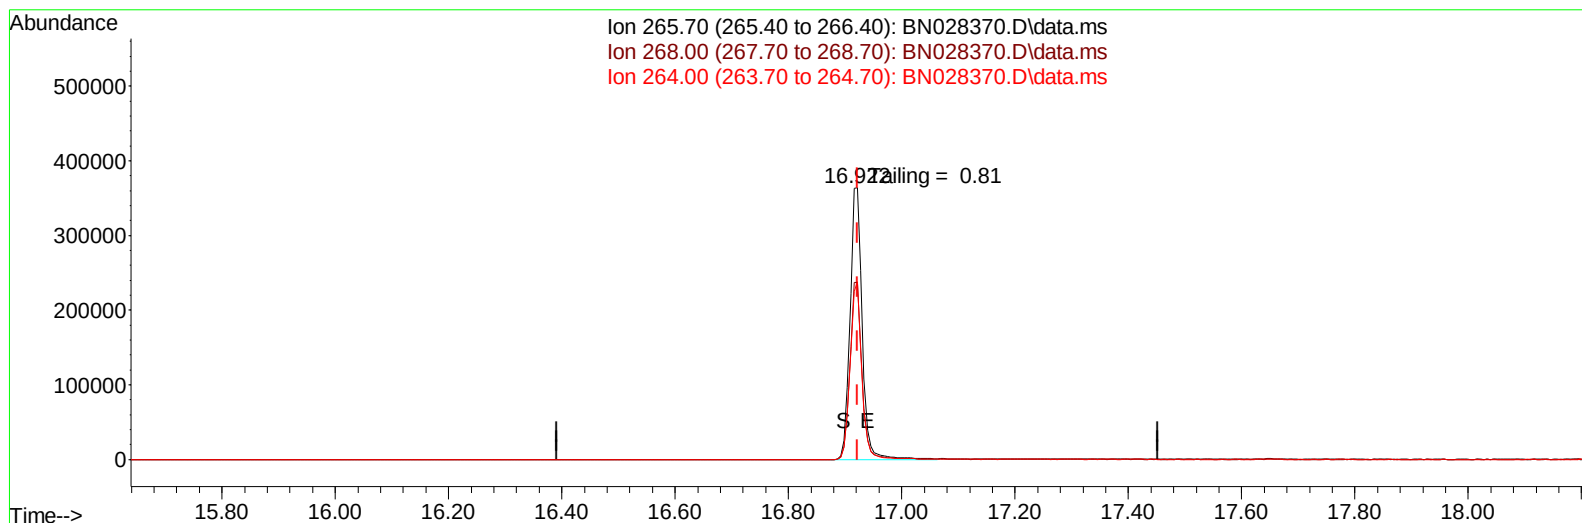

TIC: BN028370.D\data.ms

(70) Pentachlorophenol (C)

16.922min (0.000) 23264.19 ng




response 547897

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.17
264.00	61.60	65.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102423\
Data File : BN028370.D
Acq On : 24 Oct 2023 10:09
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 25 05:13:45 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 25 05:13:40 2023
Response via : Initial Calibration

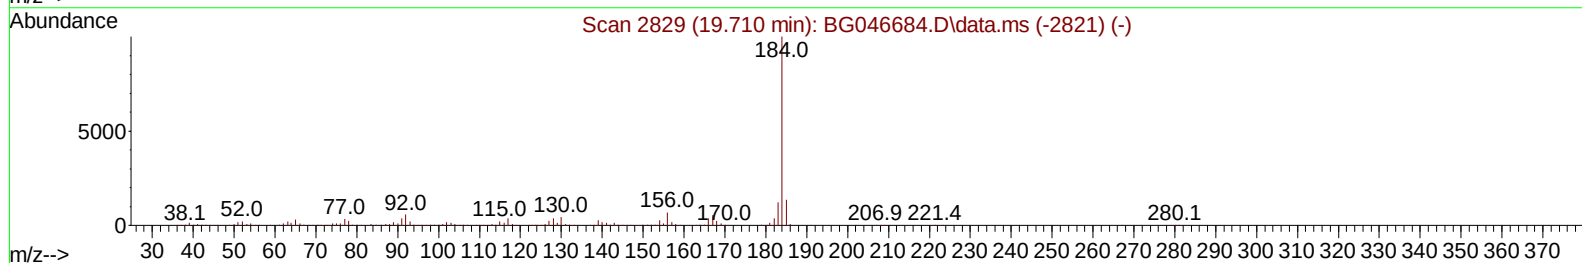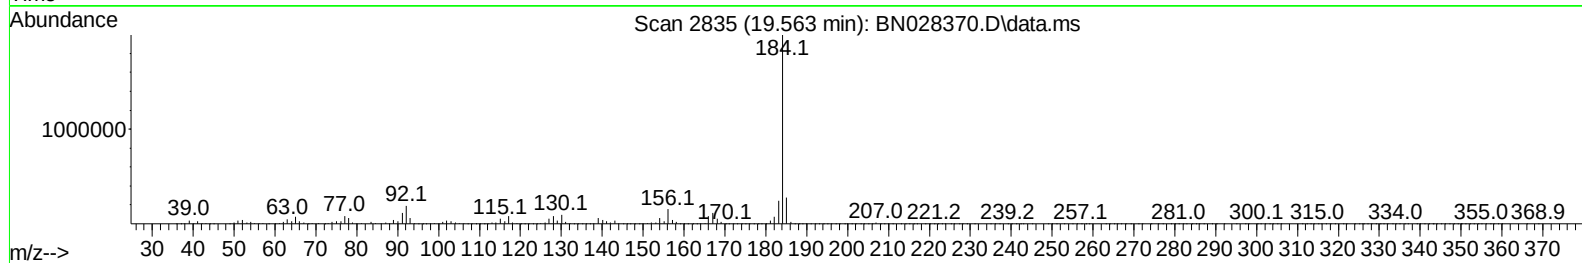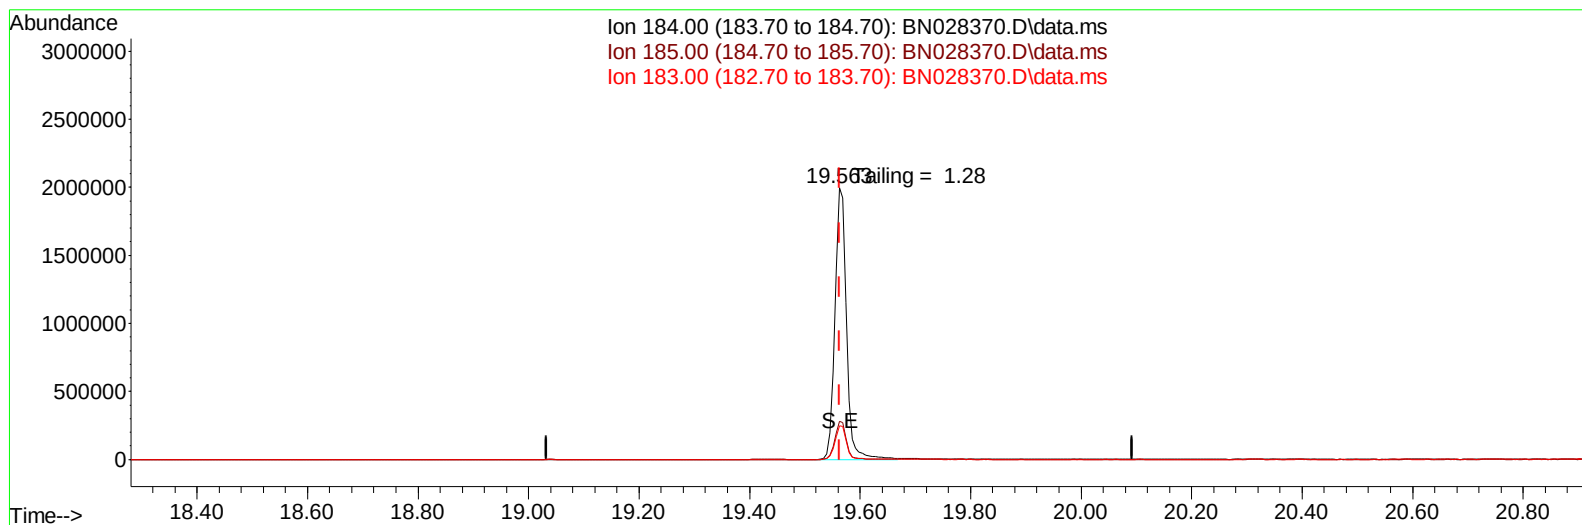

TIC: BN028370.D\data.ms

(77) Benzidine

19.563min (0.000) 675556.71 ng

response 2977873

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.04
183.00	13.20	12.35
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/24/2023	BNA_N	<u>BN028370.D</u>
Compound Name	Response	Retention Time
DDT	788530	20.751
DDD	482015	20.316
DDE	1170	19.792
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
483185	1271715	37.99

Instrument :
BNA_N
ClientSampleId :
DFTPP