


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102423\
Data File : BN028383.D
Acq On : 24 Oct 2023 19:59
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN101223.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Oct 23 15:14:08 2023

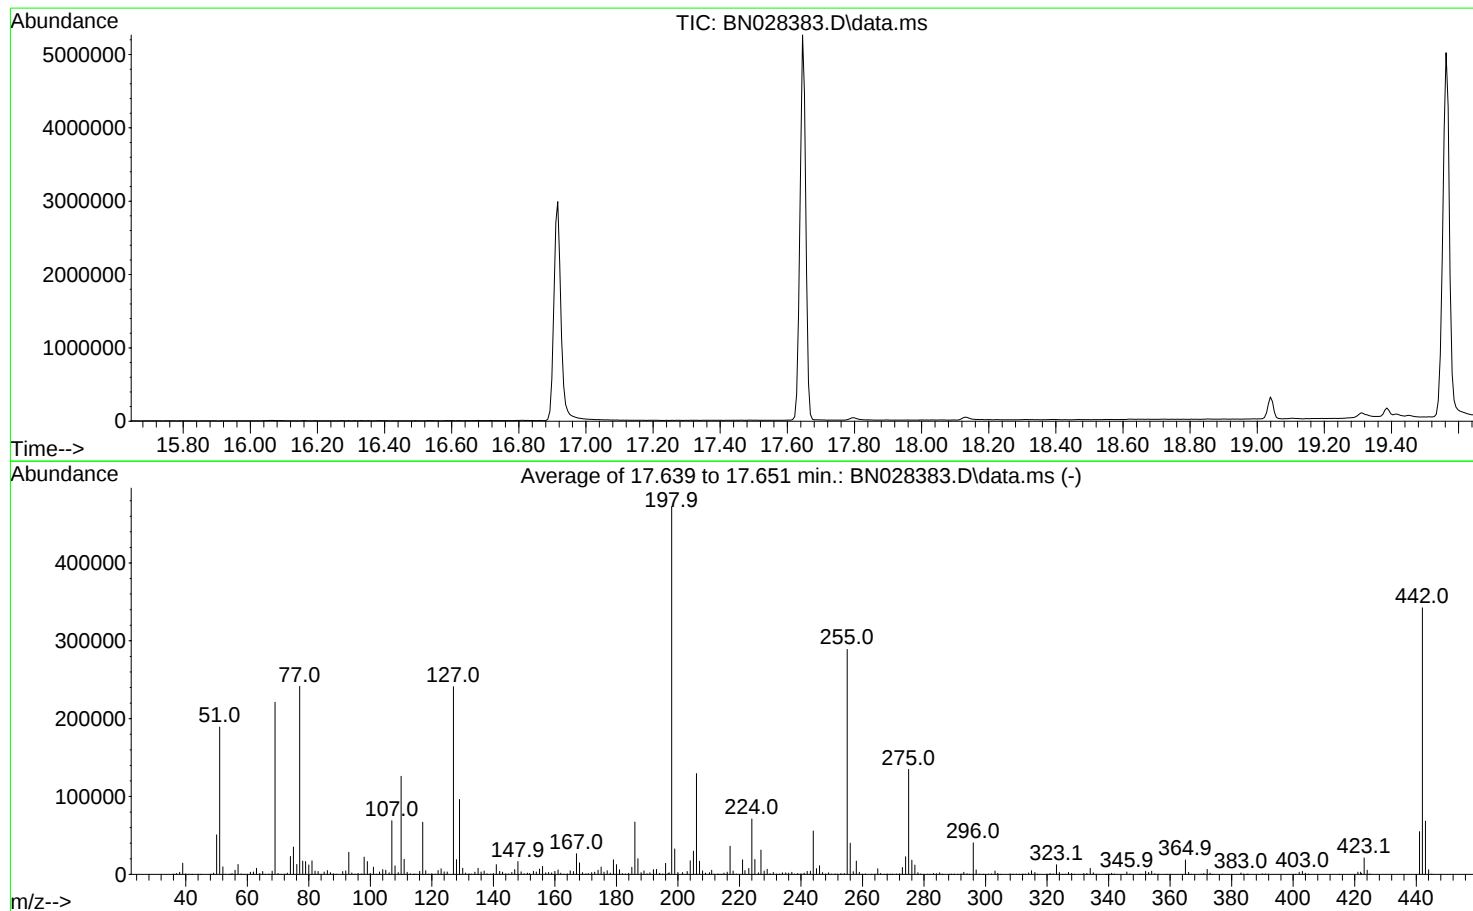




AutoFind: Scans 2508, 2509, 2510; Background Corrected with Scan 2501

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.1	189270	PASS
68	69	0.00	2	1.9	4107	PASS
69	198	0.00	100	46.8	221171	PASS
70	69	0.00	2	0.6	1301	PASS
127	198	10	80	51.0	241109	PASS
197	198	0.00	2	0.4	2085	PASS
198	198	100	100	100.0	472533	PASS
199	198	5	9	6.9	32685	PASS
275	198	10	60	28.5	134779	PASS
365	198	1	100	3.9	18428	PASS
441	198	0.01	100	11.6	54981	PASS
442	442	50	100	100.0	342464	PASS
443	442	15	24	20.0	68547	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102423\
Data File : BN028383.D
Acq On : 24 Oct 2023 19:59
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 25 05:15:04 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 25 05:13:40 2023
Response via : Initial Calibration

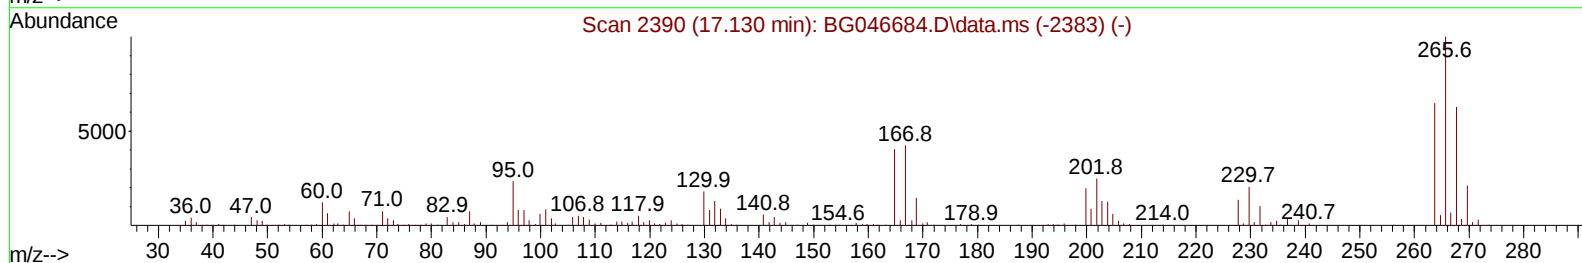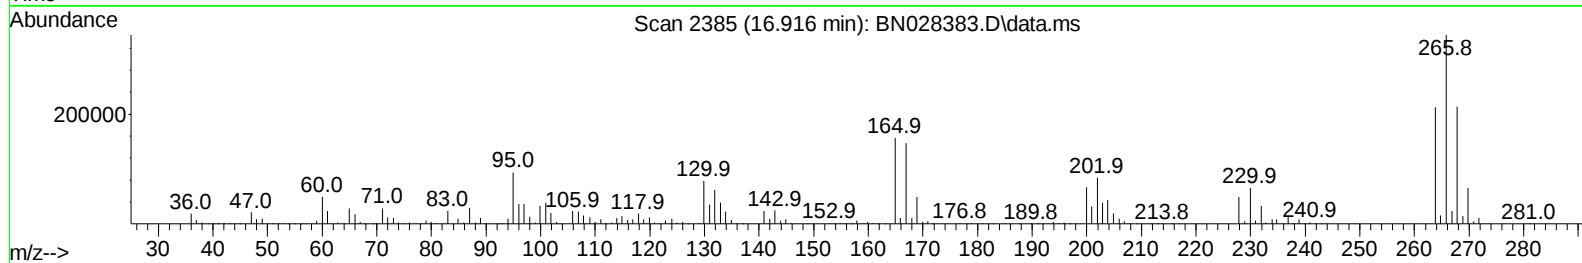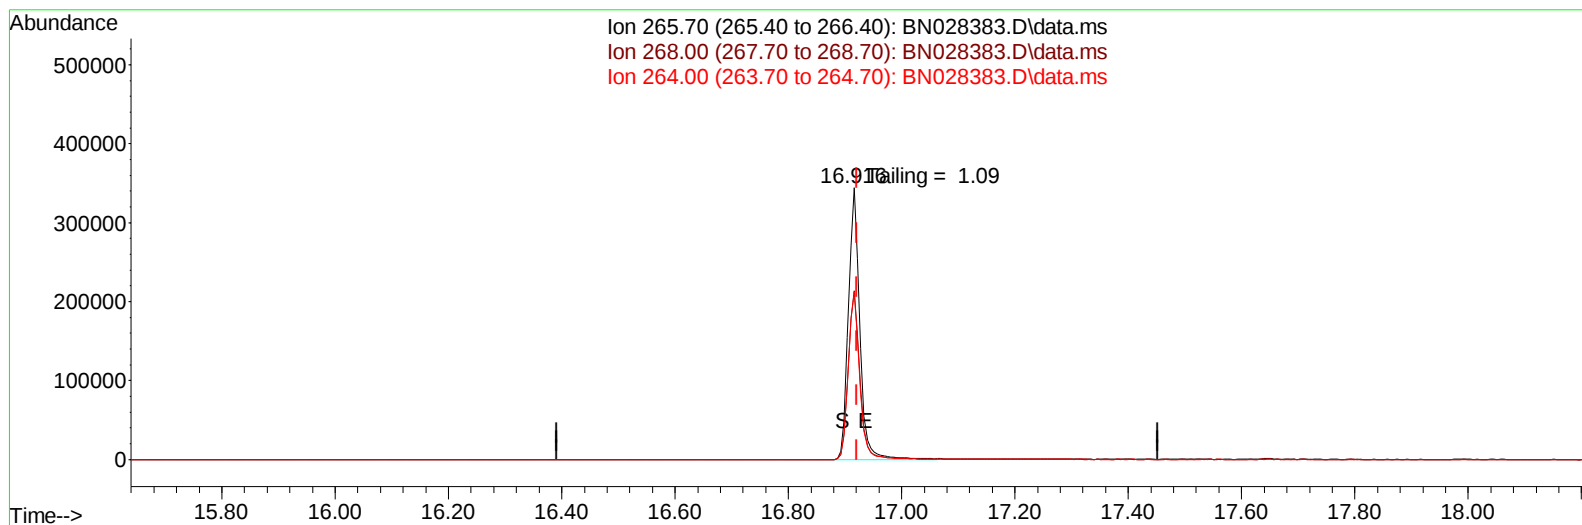

TIC: BN028383.D\data.ms

(70) Pentachlorophenol (C)

16.916min (-0.006) 19923.86 ng




response 483770

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.08
264.00	61.60	61.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102423\
 Data File : BN028383.D
 Acq On : 24 Oct 2023 19:59
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Oct 25 05:15:04 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 25 05:13:40 2023
 Response via : Initial Calibration

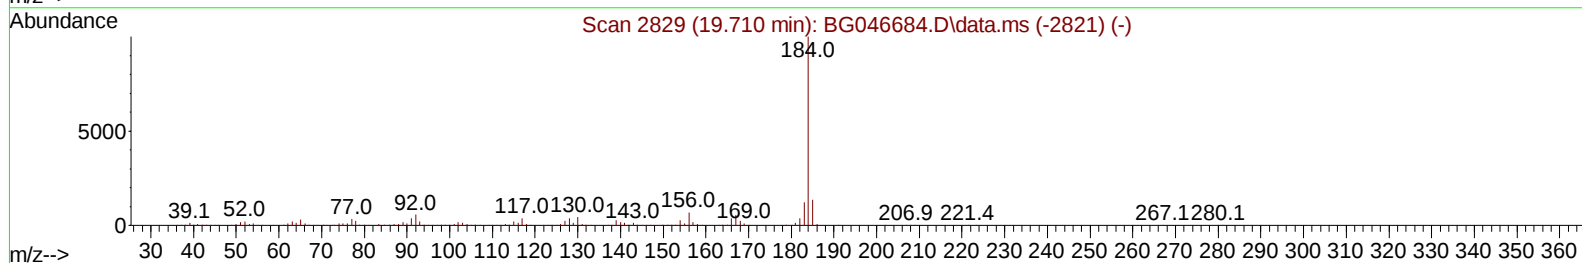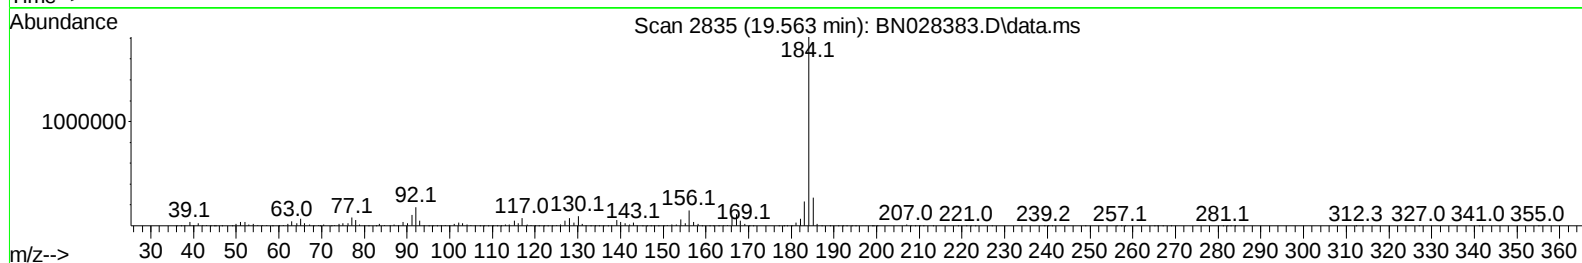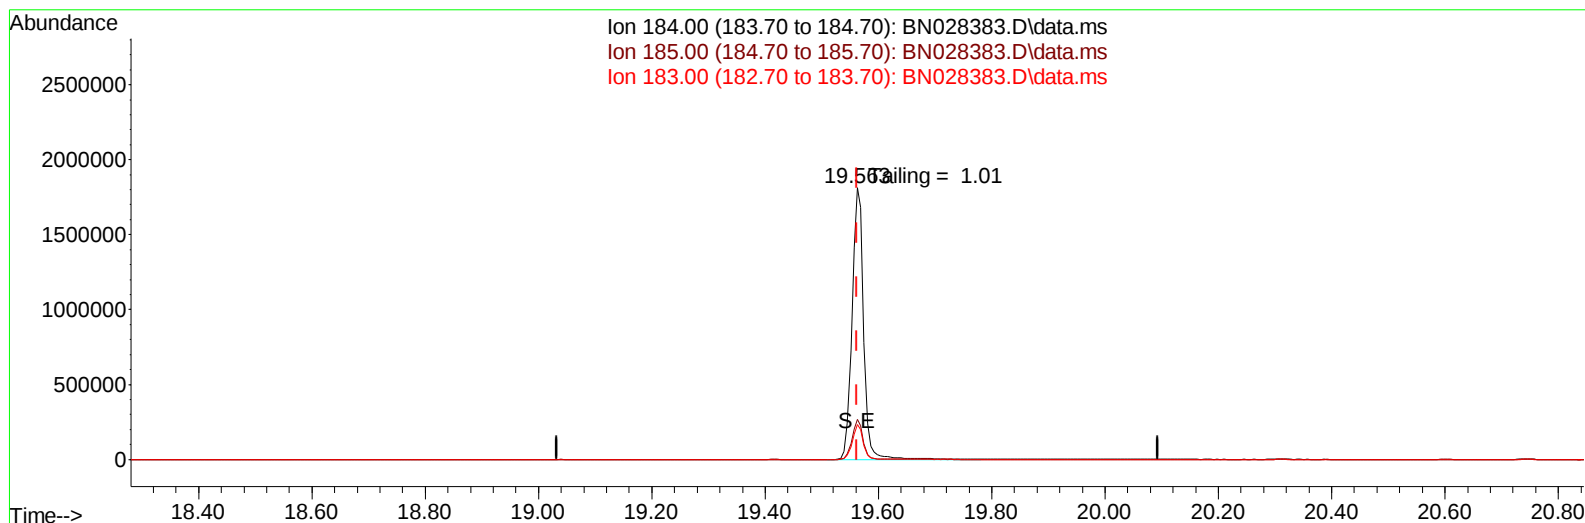

TIC: BN028383.D\data.ms

(77) Benzidine

19.563min (+ 0.000) 657411.98 ng

response 2593916

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.80
183.00	13.20	12.91
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/24/2023	BNA_N	<u>BN028383.D</u>
Compound Name	Response	Retention Time
DDT	588691	20.745
DDD	455611	20.316
DDE	1306	19.792
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
456917	1045608	43.70

Instrument :
BNA_N
ClientSampleId :
DFTPP