


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN102618\
 Data File : BN003298.D
 Acq On : 26 Oct 2018 09:16
 Operator : MJ/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN102618.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 26 15:17:57 2018

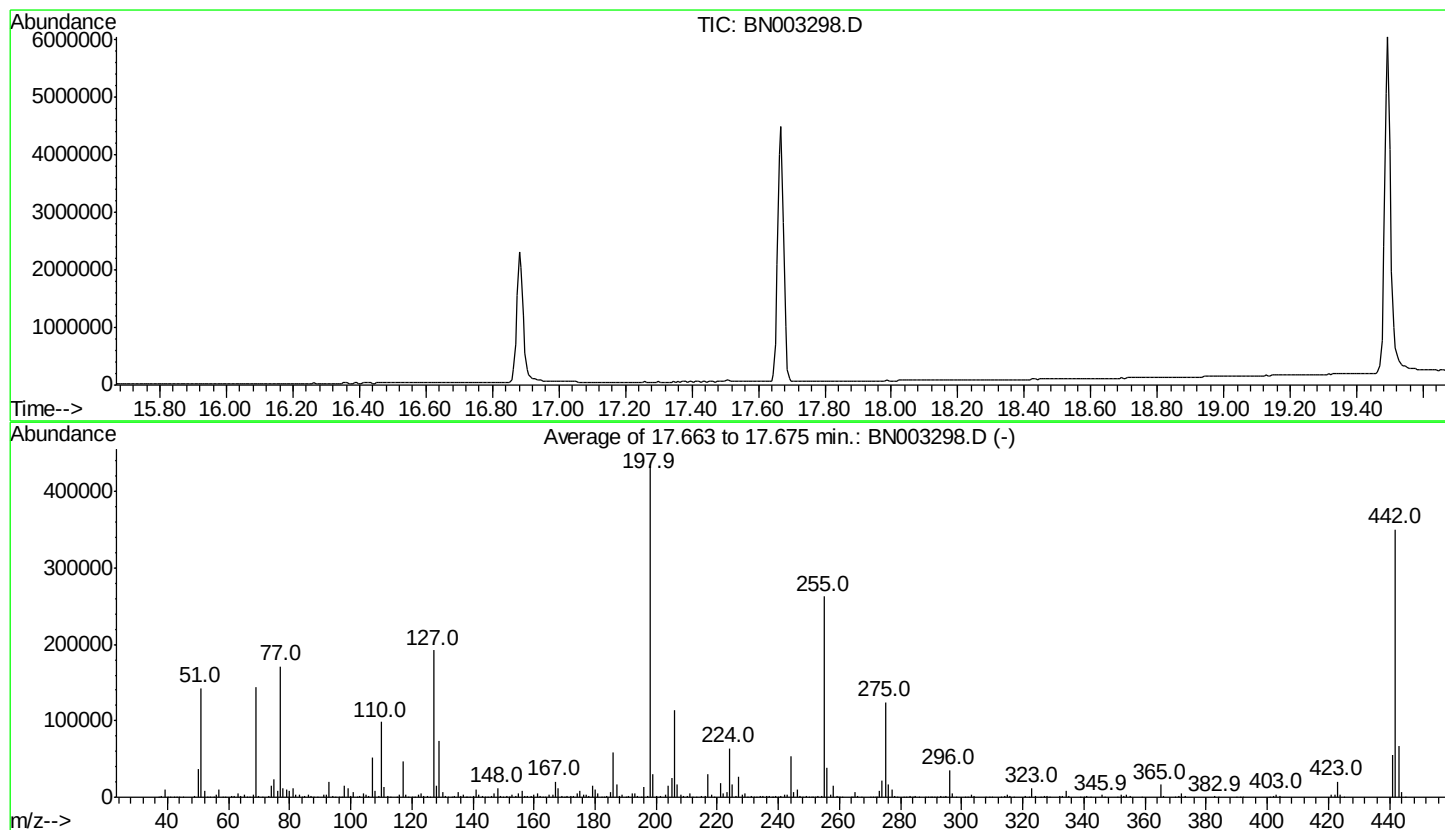

AutoFind: Scans 2495, 2496, 2497; Background Corrected with Scan 2488

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.9	142608	PASS
68	69	0.00	2	2.0	2816	PASS
69	198	0.00	100	33.1	143586	PASS
70	69	0.00	2	0.7	967	PASS
127	198	10	80	44.3	192048	PASS
197	198	0.00	2	0.4	1520	PASS
198	198	100	100	100.0	434005	PASS
199	198	5	9	6.8	29672	PASS
275	198	10	60	28.7	124445	PASS
365	198	1	100	3.7	16272	PASS
441	198	0.01	100	12.8	55597	PASS
442	198	50	100	80.8	350549	PASS
443	442	15	24	18.9	66362	PASS