


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102618\
 Data File : BN003317.D
 Acq On : 26 Oct 2018 22:24
 Operator : MJ/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN102618.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 26 15:17:57 2018

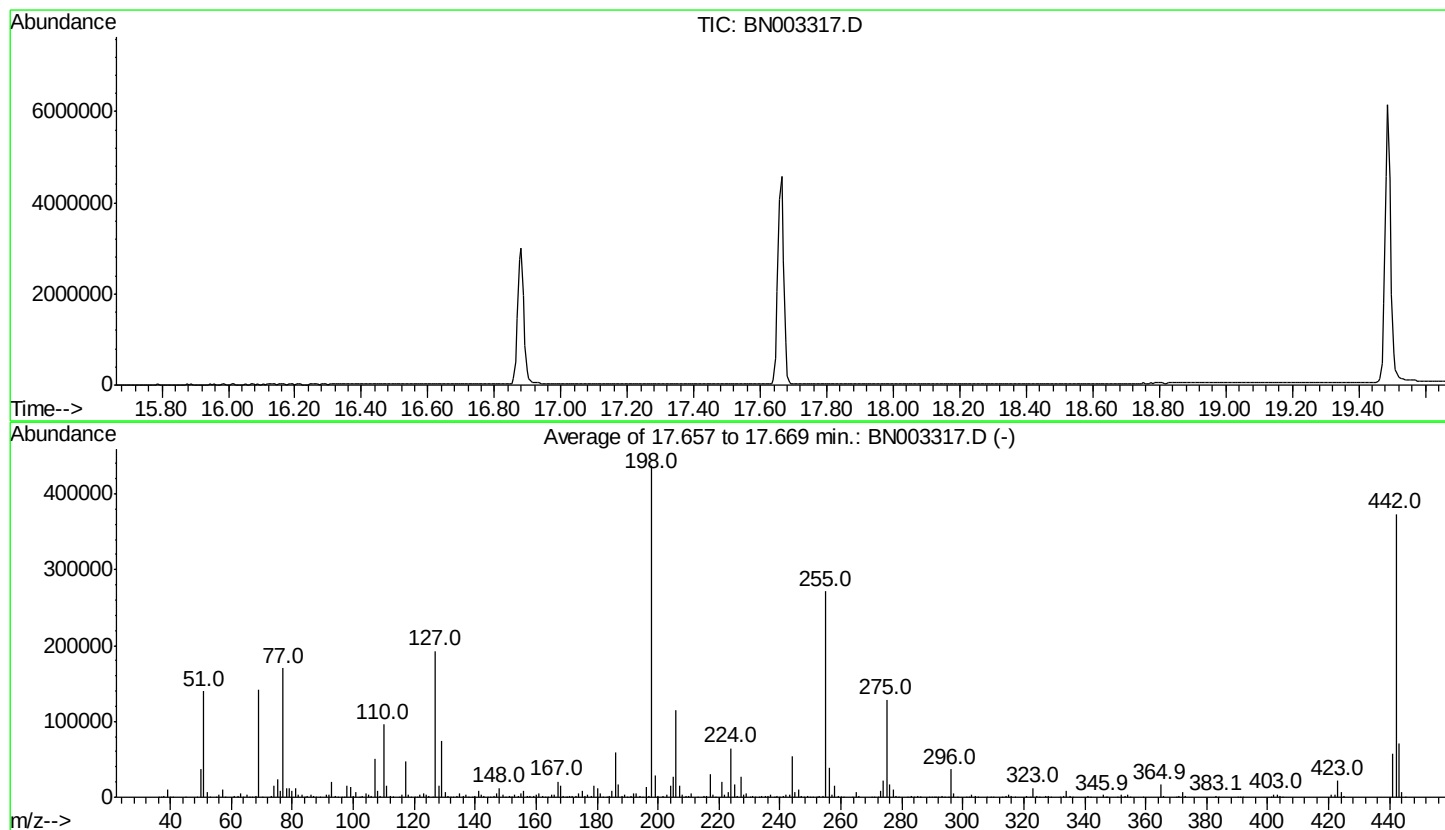

AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2487

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.0	139914	PASS
68	69	0.00	2	1.8	2543	PASS
69	198	0.00	100	32.5	142298	PASS
70	69	0.00	2	0.5	738	PASS
127	198	10	80	44.1	192880	PASS
197	198	0.00	2	0.6	2432	PASS
198	198	100	100	100.0	437226	PASS
199	198	5	9	6.7	29157	PASS
275	198	10	60	29.5	128826	PASS
365	198	1	100	3.7	16125	PASS
441	198	0.01	100	13.3	58122	PASS
442	198	50	100	85.4	373482	PASS
443	442	15	24	19.2	71690	PASS