


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102621\
Data File : BN017114.D
Acq On : 27 Oct 2021 05:47
Operator : CG/JU
Sample : M4215-01
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JDGB7

Quant Time: Oct 27 06:46:11 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN102621.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 26 15:29:15 2021
Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
10/27/2021 2:23:40 PM

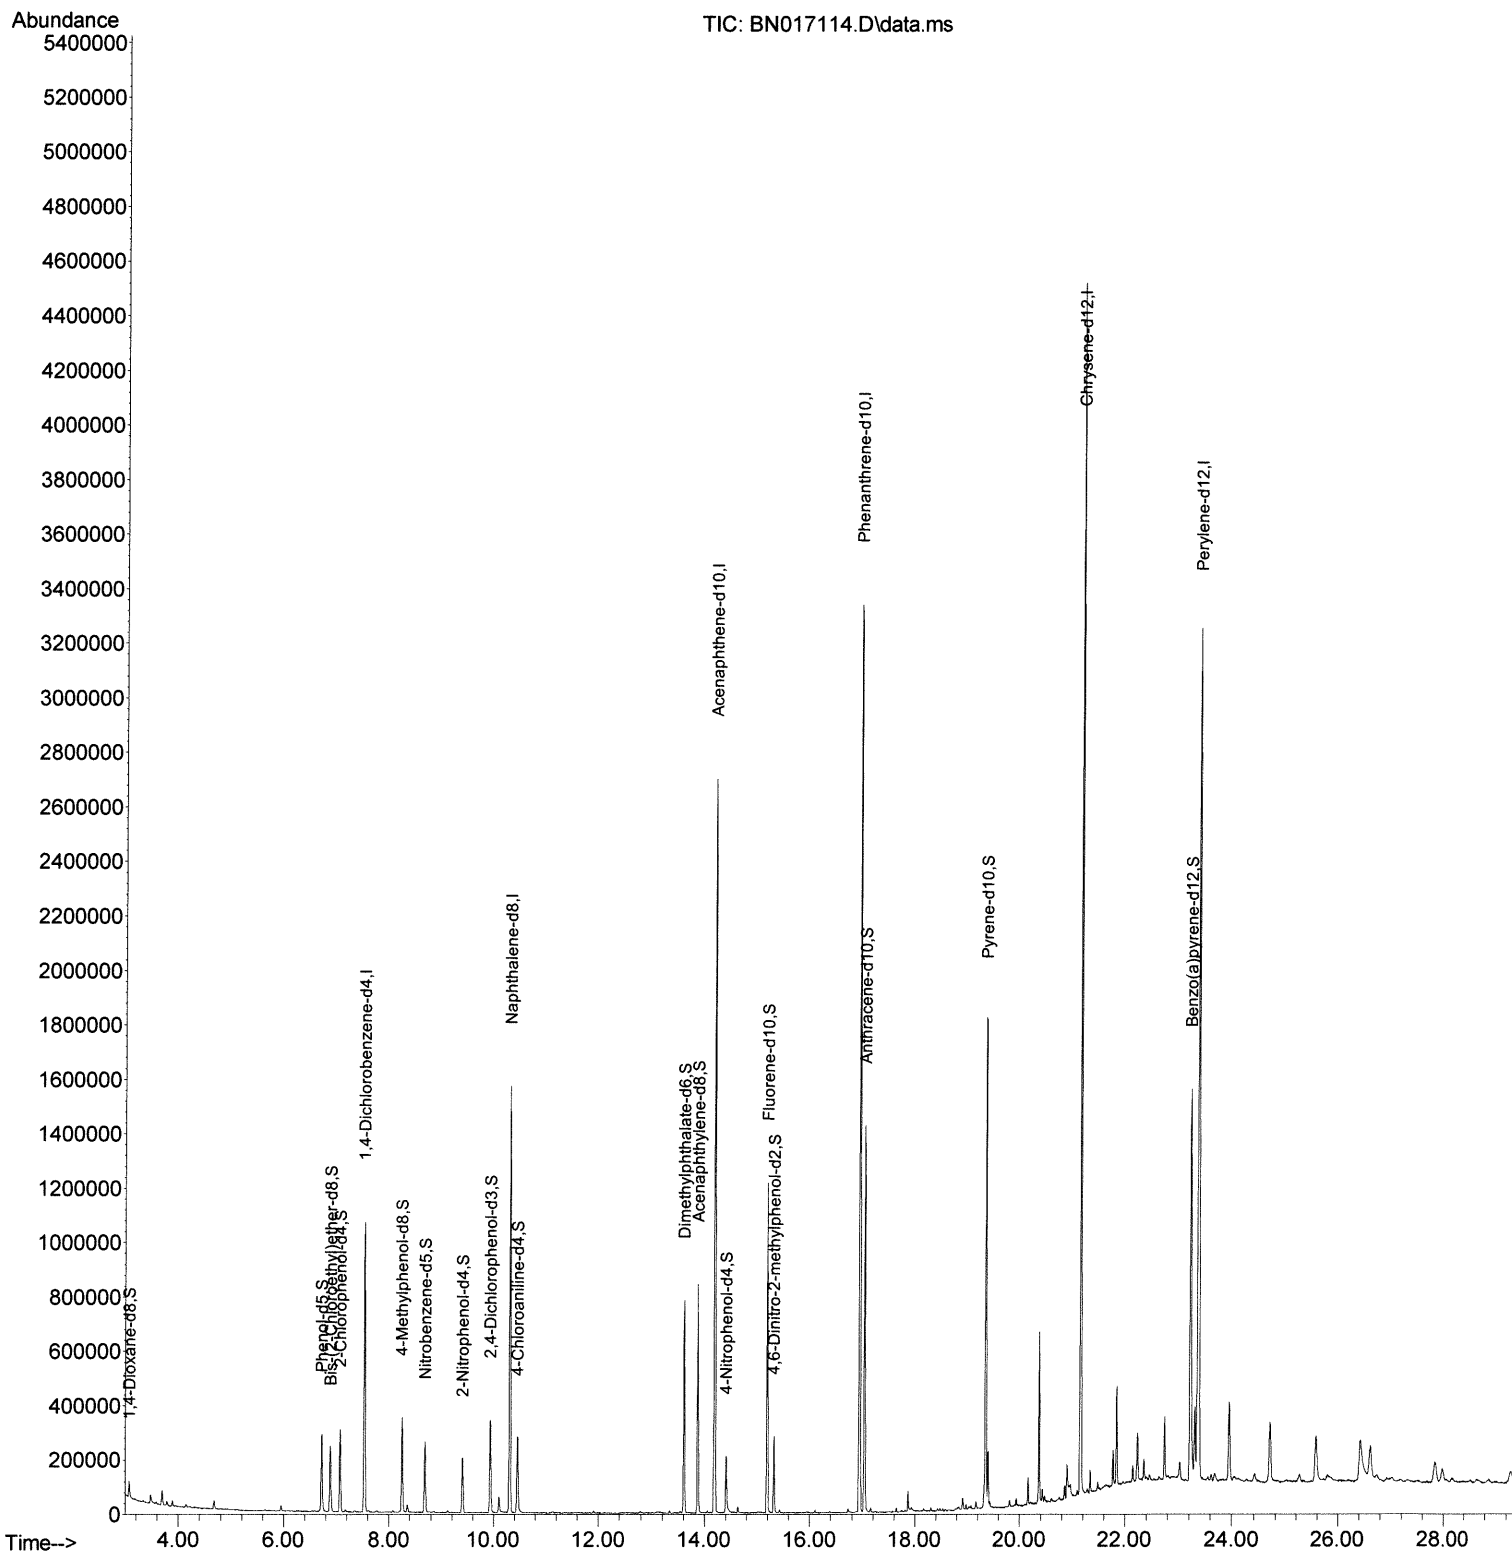


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102621\
Data File : BN017114.D
Acq On : 27 Oct 2021 05:47
Operator : CG/JU
Sample : M4215-01
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JDGB7

Manual Integrations
APPROVED

mohammad
10/27/2021 2:23:40 PM

Quant Time: Oct 27 06:46:11 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN102621.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 26 15:29:15 2021
Response via : Initial Calibration

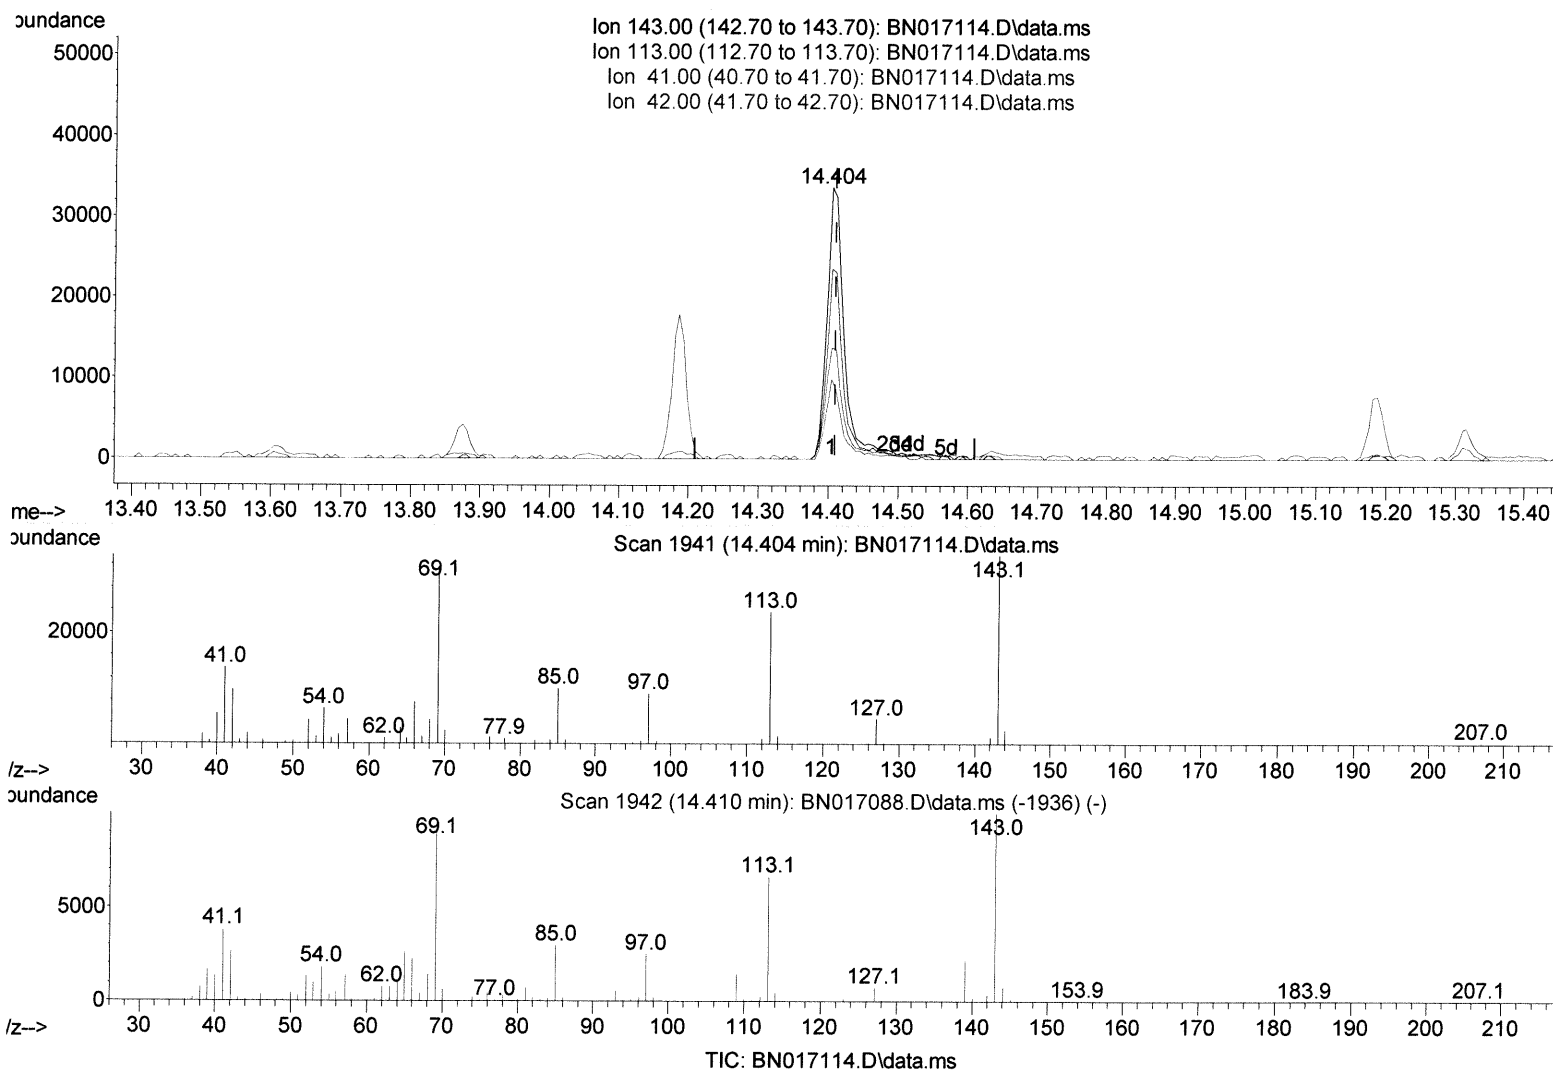

(54) 4-Nitrophenol-d4 (S)

14.404min (-0.006) 4.15 ng/ul

response 54372

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	66.20	70.26
41.00	38.00	40.96
42.00	26.30	29.29




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102621\
 Data File : BN017114.D
 Acq On : 27 Oct 2021 05:47
 Operator : CG/JU
 Sample : M4215-01
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JDGB7

Manual Integrations
 APPROVED

mohammad
 10/27/2021 2:23:40 PM

Quant Time: Oct 27 06:46:11 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN102621.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 26 15:29:15 2021
 Response via : Initial Calibration

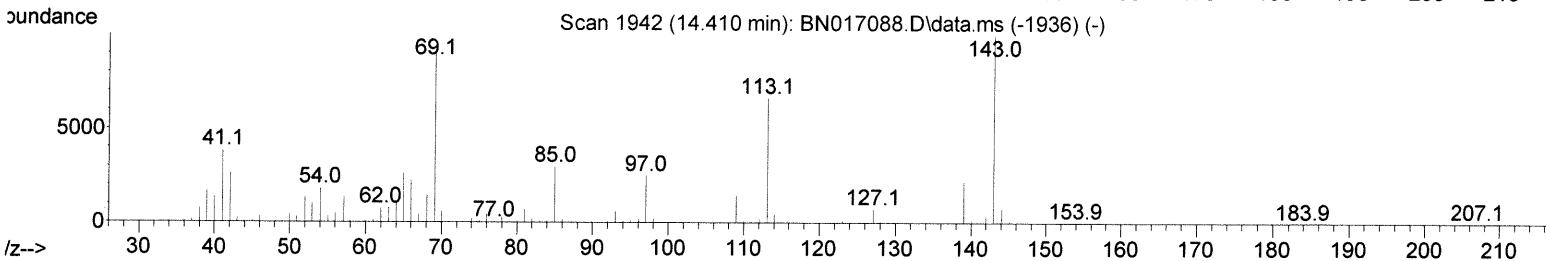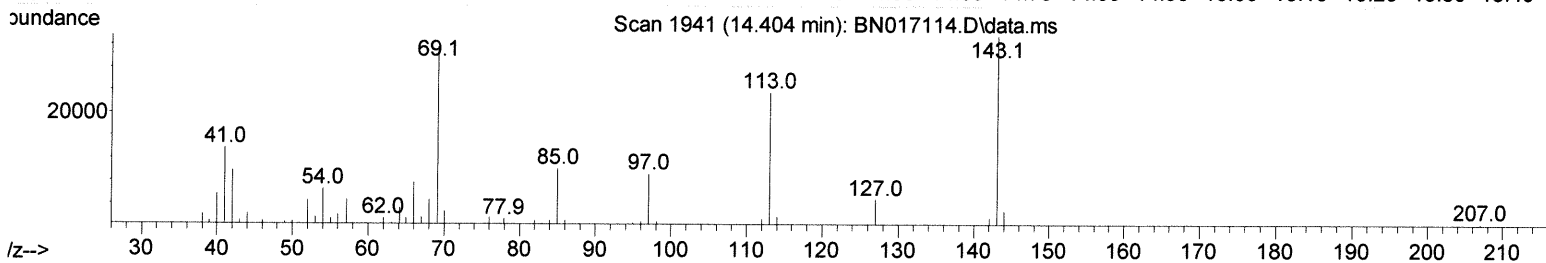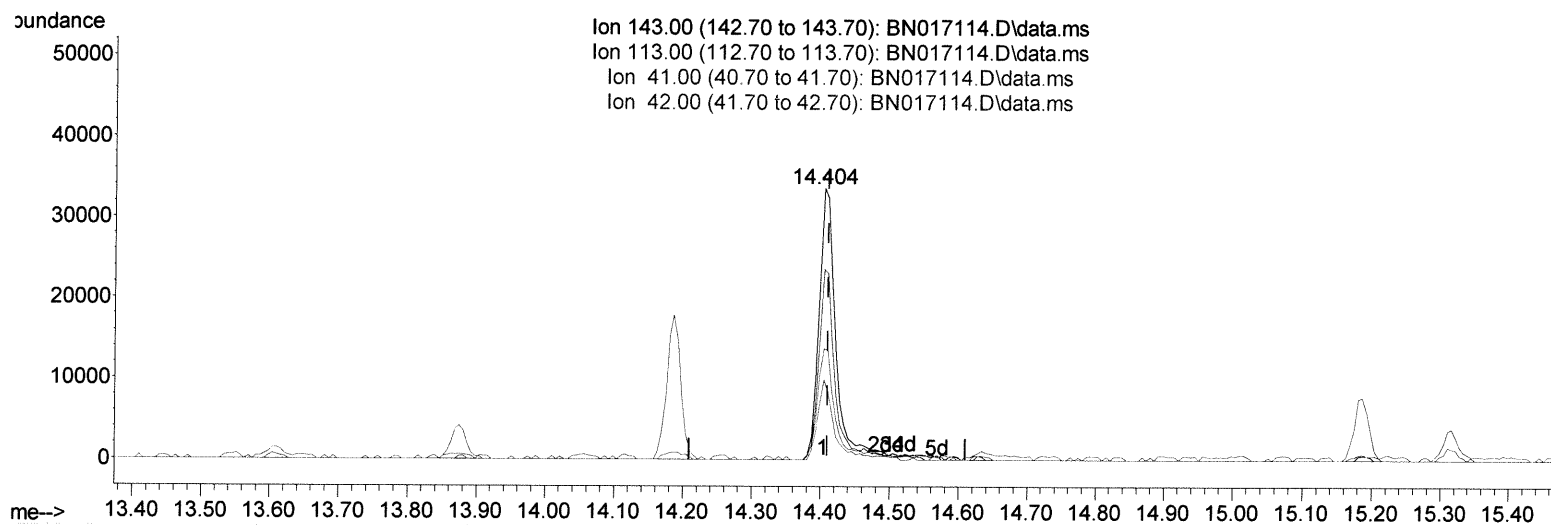

TIC: BN017114.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.404min (-0.006) 4.31 ng/ul m 10/29/21 JU

response 56466

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	66.20	70.26
41.00	38.00	40.96
42.00	26.30	29.29

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102621\
 Data File : BN017114.D
 Acq On : 27 Oct 2021 05:47
 Operator : CG/JU
 Sample : M4215-01
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JDGB7

Manual Integrations
 APPROVED

mohammad
 10/27/2021 2:23:40 PM

Quant Time: Oct 27 06:46:11 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN102621.M
 Quant Title : SVOA CALIBRATION
 Last Update : Tue Oct 26 15:29:15 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.534	152	280544	20.000	ng/ul	0.00
20) Naphthalene-d8	10.310	136	1300972	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.187	164	886660	20.000	ng/ul	0.00
64) Phenanthrene-d10	16.939	188	1951561	20.000	ng/ul	0.00
79) Chrysene-d12	21.157	240	2016953	20.000	ng/ul	0.00
88) Perylene-d12	23.368	264	2112984	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.069	96	28609	3.694	ng/uL	0.00
4) Pyridine-d5	3.475	84	18136	0.874	ng/ul	0.01
7) Phenol-d5	6.722	99	160414	6.153	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.887	67	107556	6.951	ng/ul	0.00
11) 2-Chlorophenol-d4	7.069	132	138386	6.750	ng/ul	0.00
15) 4-Methylphenol-d8	8.246	113	130685	6.141	ng/ul	0.00
21) Nitrobenzene-d5	8.687	128	61289	6.083	ng/ul	0.00
24) 2-Nitrophenol-d4	9.399	143	65652	5.886	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.934	165	123468	6.042	ng/ul	0.00
31) 4-Chloroaniline-d4	10.457	131	157927	5.189	ng/ul	0.00
46) Dimethylphthalate-d6	13.610	166	504323	7.598	ng/ul	0.00
49) Acenaphthylene-d8	13.875	160	576055	6.884	ng/ul	0.00
54) 4-Nitrophenol-d4	14.404	143	56466m	4.311	ng/ul	0.00
60) Fluorene-d10	15.186	176	451466	7.963	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.316	200	52977	4.192	ng/ul	0.00
73) Anthracene-d10	17.039	188	757041	8.035	ng/ul	0.00
81) Pyrene-d10	19.351	212	964384	8.153	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.221	264	978143	8.710	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed