

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102621\
 Data File : BN017095.D
 Acq On : 26 Oct 2021 17:37
 Operator : CG/JU
 Sample : M4318-07
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 P020-TW001-02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN102621.M
 Title : SVOA CALIBRATION

Signal : TIC: BN017095.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.070	11	14	26	rVB	82346	120474	1.09%	0.124%
2	3.470	78	82	96	rBV	156424	260823	2.36%	0.269%
3	3.699	115	121	127	rVB2	51474	84432	0.76%	0.087%
4	3.787	132	136	143	rVB	20891	30731	0.28%	0.032%
5	3.887	150	153	159	rVB3	18541	27032	0.24%	0.028%
6	4.681	284	288	295	rVB2	7772	13845	0.13%	0.014%
7	5.952	499	504	509	rVB	16482	23591	0.21%	0.024%
8	6.722	629	635	646	rBV	338645	511553	4.62%	0.528%
9	6.887	656	663	677	rBV	1203441	1855234	16.77%	1.914%
10	7.069	688	694	707	rVV	1230652	1868329	16.88%	1.928%
11	7.534	766	773	782	rBV	1151544	1781231	16.10%	1.838%
12	8.252	888	895	907	rBV	975127	1492139	13.48%	1.540%
13	8.687	962	969	980	rBV	1445426	2269588	20.51%	2.342%
14	8.822	987	992	997	rBV2	8262	12763	0.12%	0.013%
15	9.405	1084	1091	1102	rBV	1200707	1871735	16.91%	1.931%
16	9.940	1175	1182	1202	rBV	1643787	2690725	24.32%	2.776%
17	10.310	1237	1245	1255	rBV	1737387	2823047	25.51%	2.913%
18	10.457	1263	1270	1287	rBV	1404077	2355795	21.29%	2.431%
19	11.910	1511	1517	1525	rBV	32380	52748	0.48%	0.054%
20	13.616	1800	1807	1816	rBV	3528861	4940554	44.65%	5.098%
21	13.881	1845	1852	1868	rBV	4067797	6003231	54.25%	6.194%
22	14.187	1898	1904	1913	rBV	2730538	4018782	36.32%	4.147%
23	14.410	1936	1942	1955	rBV	295805	462271	4.18%	0.477%
24	14.634	1974	1980	1984	rVB3	14219	18512	0.17%	0.019%
25	15.192	2068	2075	2089	rBV	5521011	7815277	70.62%	8.064%
26	15.322	2090	2097	2111	rVV	2019024	2684534	24.26%	2.770%
27	15.428	2111	2115	2120	rVB	35915	49143	0.44%	0.051%
28	15.939	2199	2202	2205	rBV2	13558	16120	0.15%	0.017%
29	15.969	2205	2207	2215	rVB7	7143	11183	0.10%	0.012%
30	16.734	2332	2337	2341	rBV2	36345	49781	0.45%	0.051%
31	16.786	2341	2346	2352	rVB3	12739	22404	0.20%	0.023%
32	16.945	2366	2373	2383	rBV	3594041	4899132	44.27%	5.055%
33	17.045	2383	2390	2407	rVV2	6502963	9167334	82.84%	9.459%
34	17.275	2423	2429	2434	rBV4	7285	12544	0.11%	0.013%
35	17.333	2435	2439	2442	rBV2	10237	14091	0.13%	0.015%
36	17.392	2446	2449	2454	rVB5	8761	12610	0.11%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102621\
 Data File : BN017095.D
 Acq On : 26 Oct 2021 17:37
 Operator : CG/JU
 Sample : M4318-07
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 P020-TW001-02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN102621.M
 Title : SVOA CALIBRATION

37	17.475	2459	2463	2468	rVV	56007	68918	0.62%	0.071%
38	17.651	2489	2493	2496	rVB3	14810	19567	0.18%	0.020%
39	17.757	2507	2511	2515	rBV5	12340	23140	0.21%	0.024%
40	17.869	2526	2530	2535	rBV4	33047	49110	0.44%	0.051%
41	17.922	2536	2539	2545	rVB4	14266	25678	0.23%	0.026%
42	17.981	2547	2549	2552	rBV3	11631	15958	0.14%	0.016%
43	18.069	2561	2564	2568	rVB5	11093	13138	0.12%	0.014%
44	18.122	2570	2573	2577	rVB5	12608	17073	0.15%	0.018%
45	18.175	2577	2582	2586	rBV	88326	112514	1.02%	0.116%
46	18.428	2623	2625	2628	rBV4	16395	18905	0.17%	0.020%
47	18.639	2658	2661	2665	rVB2	45707	56616	0.51%	0.058%
48	18.751	2677	2680	2684	rVB4	21066	26531	0.24%	0.027%
49	18.816	2687	2691	2696	rBV	84458	103281	0.93%	0.107%
50	18.916	2704	2708	2715	rVB2	94771	132462	1.20%	0.137%
51	18.980	2715	2719	2725	rBV	137499	211836	1.91%	0.219%
52	19.039	2726	2729	2733	rBV3	30215	41481	0.37%	0.043%
53	19.157	2745	2749	2752	rBV3	36995	61041	0.55%	0.063%
54	19.351	2776	2782	2788	rBV	7668990	10648504	96.23%	10.987%
55	19.398	2788	2790	2794	rVB	65870	70350	0.64%	0.073%
56	19.575	2816	2820	2822	rBV3	45751	75167	0.68%	0.078%
57	19.939	2878	2882	2885	rBV	77956	93897	0.85%	0.097%
58	20.122	2910	2913	2918	rBV3	67509	104625	0.95%	0.108%
59	20.233	2929	2932	2934	rBV2	52015	71970	0.65%	0.074%
60	20.604	2992	2995	3005	rVB3	73899	167928	1.52%	0.173%
61	21.057	3068	3072	3077	rBV	131397	245357	2.22%	0.253%
62	21.157	3084	3089	3095	rBV	4494319	5484793	49.56%	5.659%
63	21.480	3141	3144	3152	rVB2	158200	255433	2.31%	0.264%
64	22.739	3355	3358	3364	rVB	138941	179889	1.63%	0.186%
65	23.233	3434	3442	3450	rBV2	5866913	11066034	100.00%	11.418%
66	23.304	3451	3454	3458	rVV2	225837	382803	3.46%	0.395%
67	23.368	3458	3465	3479	rVB	3141875	5918187	53.48%	6.106%
68	23.957	3560	3565	3573	rVB2	185176	394442	3.56%	0.407%
69	24.704	3687	3692	3706	rVB	172539	419715	3.79%	0.433%



Sum of corrected areas: 96919661

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102621\
Data File : BN017095.D
Acq On : 26 Oct 2021 17:37
Operator : CG/JU
Sample : M4318-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
P020-TW001-02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN102621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

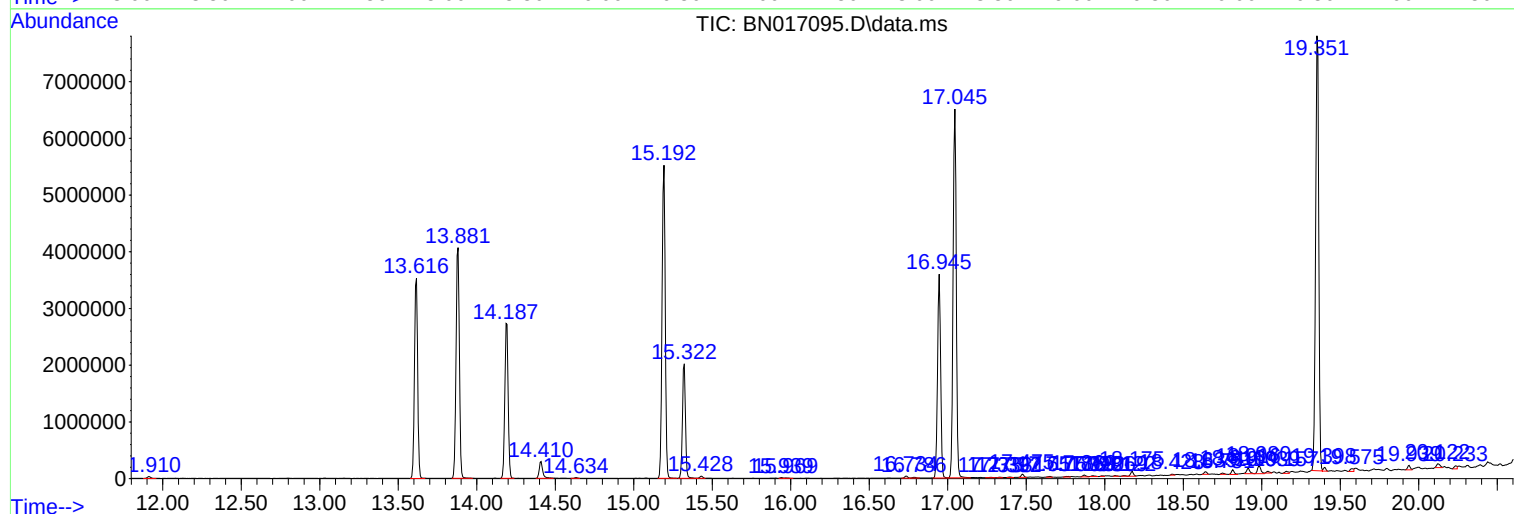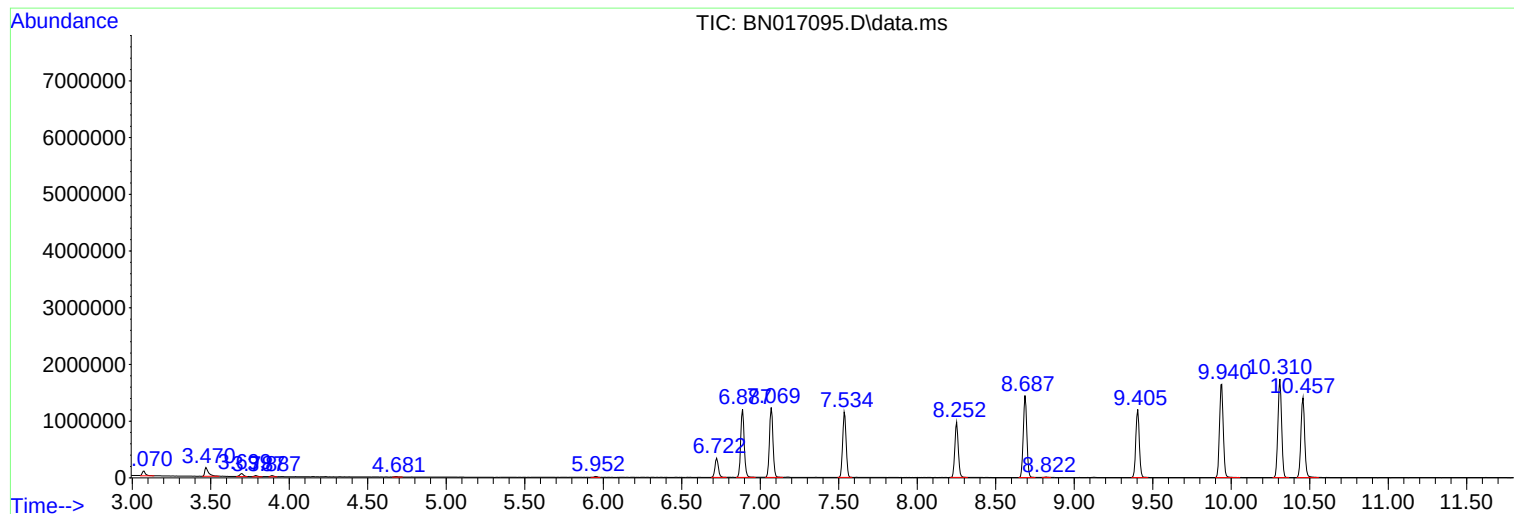

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102621\
Data File : BN017095.D
Acq On : 26 Oct 2021 17:37
Operator : CG/JU
Sample : M4318-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
P020-TW001-02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN102621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102621\
Data File : BN017095.D
Acq On : 26 Oct 2021 17:37
Operator : CG/JU
Sample : M4318-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
P020-TW001-02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN102621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------