

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102621\
 Data File : BN017096.D
 Acq On : 26 Oct 2021 18:14
 Operator : CG/JU
 Sample : M4318-08
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 P023-TW001-02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN102621.M
 Title : SVOA CALIBRATION

Signal : TIC: BN017096.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.075	11	15	26	rVB	68315	108667	0.89%	0.102%
2	3.470	78	82	98	rBV	306073	534759	4.37%	0.503%
3	3.693	115	120	130	rVV	49138	85370	0.70%	0.080%
4	3.787	132	136	146	rVV	23048	39751	0.33%	0.037%
5	3.887	149	153	160	rVB4	18527	31204	0.26%	0.029%
6	5.952	500	504	512	rVB	17033	25711	0.21%	0.024%
7	6.722	629	635	651	rVB	337907	533028	4.36%	0.502%
8	6.887	656	663	674	rBV	1271787	1949626	15.95%	1.835%
9	7.069	687	694	708	rVB	1250752	1936092	15.84%	1.822%
10	7.534	767	773	781	rBV	1276639	1991987	16.30%	1.874%
11	8.252	888	895	908	rBV	966320	1521895	12.45%	1.432%
12	8.687	962	969	980	rBV	1551938	2412405	19.74%	2.270%
13	9.128	1038	1044	1049	rVB2	11145	17213	0.14%	0.016%
14	9.404	1083	1091	1106	rBV	1269581	1997810	16.34%	1.880%
15	9.940	1175	1182	1192	rBV	1745706	2858091	23.38%	2.689%
16	10.110	1206	1211	1220	rBV	23037	45549	0.37%	0.043%
17	10.310	1237	1245	1254	rBV	1926876	3130014	25.61%	2.945%
18	10.457	1261	1270	1289	rBV	1685808	2846323	23.29%	2.678%
19	11.910	1510	1517	1524	rBV2	35266	57553	0.47%	0.054%
20	11.981	1524	1529	1537	rBV4	9913	23252	0.19%	0.022%
21	13.028	1703	1707	1712	rVB5	11341	16728	0.14%	0.016%
22	13.616	1800	1807	1817	rBV	3735450	5215249	42.67%	4.907%
23	13.881	1844	1852	1870	rBV	4282684	6280506	51.38%	5.910%
24	14.116	1888	1892	1896	rVB2	14951	18860	0.15%	0.018%
25	14.187	1898	1904	1923	rVB	3023224	4535653	37.11%	4.268%
26	14.410	1936	1942	1952	rBV	311990	488752	4.00%	0.460%
27	14.634	1974	1980	1985	rBV3	11122	17124	0.14%	0.016%
28	15.075	2051	2055	2061	rVB	26775	33120	0.27%	0.031%
29	15.192	2068	2075	2090	rBV	5732313	8095665	66.23%	7.618%
30	15.322	2090	2097	2110	rVV	2161513	2929321	23.96%	2.756%
31	15.428	2110	2115	2119	rVV	41492	60438	0.49%	0.057%
32	15.481	2119	2124	2128	rVB5	9367	18520	0.15%	0.017%
33	15.634	2145	2150	2155	rBV6	10213	17088	0.14%	0.016%
34	15.892	2187	2194	2198	rBV6	8639	19958	0.16%	0.019%
35	15.939	2198	2202	2205	rBV	42129	54566	0.45%	0.051%
36	16.104	2225	2230	2235	rBV5	8777	15670	0.13%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102621\
 Data File : BN017096.D
 Acq On : 26 Oct 2021 18:14
 Operator : CG/JU
 Sample : M4318-08
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 P023-TW001-02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN102621.M
 Title : SVOA CALIBRATION

37	16.733	2332	2337	2341	rBV	56154	73751	0.60%	0.069%
38	16.786	2343	2346	2353	rVB3	18599	29814	0.24%	0.028%
39	16.945	2367	2373	2383	rBV	4050950	5561563	45.50%	5.233%
40	17.045	2383	2390	2400	rBV	6901773	9525889	77.93%	8.963%
41	17.475	2459	2463	2469	rBV2	39766	50414	0.41%	0.047%
42	17.651	2487	2493	2497	rVB3	53335	68992	0.56%	0.065%
43	17.869	2526	2530	2535	rBV	68494	92926	0.76%	0.087%
44	17.939	2540	2542	2546	rVB	14744	14461	0.12%	0.014%
45	18.169	2577	2581	2585	rVB2	33191	42321	0.35%	0.040%
46	18.816	2687	2691	2692	rBV2	25303	28963	0.24%	0.027%
47	18.910	2703	2707	2713	rVB	95756	130666	1.07%	0.123%
48	18.980	2714	2719	2724	rBV	109782	160514	1.31%	0.151%
49	19.163	2747	2750	2754	rBV5	19169	23814	0.19%	0.022%
50	19.351	2772	2782	2788	rBV	8369056	11324425	92.64%	10.656%
51	19.398	2788	2790	2793	rVB	28812	29279	0.24%	0.028%
52	19.627	2825	2829	2834	rVB	66292	76201	0.62%	0.072%
53	19.939	2878	2882	2884	rBV	22922	26967	0.22%	0.025%
54	20.245	2930	2934	2935	rBV3	11512	13550	0.11%	0.013%
55	20.310	2942	2945	2950	rVB4	24286	27634	0.23%	0.026%
56	20.374	2953	2956	2961	rVV5	22258	32038	0.26%	0.030%
57	20.439	2964	2967	2971	rVB2	31603	34890	0.29%	0.033%
58	20.904	3042	3046	3053	rBV	88012	184340	1.51%	0.173%
59	21.098	3077	3079	3083	rVB2	19412	19639	0.16%	0.018%
60	21.157	3083	3089	3101	rBV	4953670	6448492	52.75%	6.068%
61	21.345	3117	3121	3129	rBV2	58005	77637	0.64%	0.073%
62	21.774	3190	3194	3198	rBV	91762	110532	0.90%	0.104%
63	22.233	3268	3272	3280	rVB	150647	212577	1.74%	0.200%
64	22.357	3288	3293	3300	rBV	369451	469796	3.84%	0.442%
65	22.739	3353	3358	3364	rBV	204259	304196	2.49%	0.286%
66	23.233	3433	3442	3450	rBV2	6231654	12223647	100.00%	11.502%
67	23.304	3450	3454	3458	rVV	275678	487662	3.99%	0.459%
68	23.368	3458	3465	3481	rVB2	3850790	6880108	56.29%	6.474%
69	23.951	3559	3564	3572	rVB	231040	448696	3.67%	0.422%
70	24.704	3686	3692	3701	rVB2	206753	455571	3.73%	0.429%
71	25.580	3834	3841	3852	rVB2	138450	361206	2.95%	0.340%
72	26.609	4011	4016	4026	rVB2	90176	258701	2.12%	0.243%


Sum of corrected areas: 106275390

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102621\
Data File : BN017096.D
Acq On : 26 Oct 2021 18:14
Operator : CG/JU
Sample : M4318-08
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
P023-TW001-02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN102621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

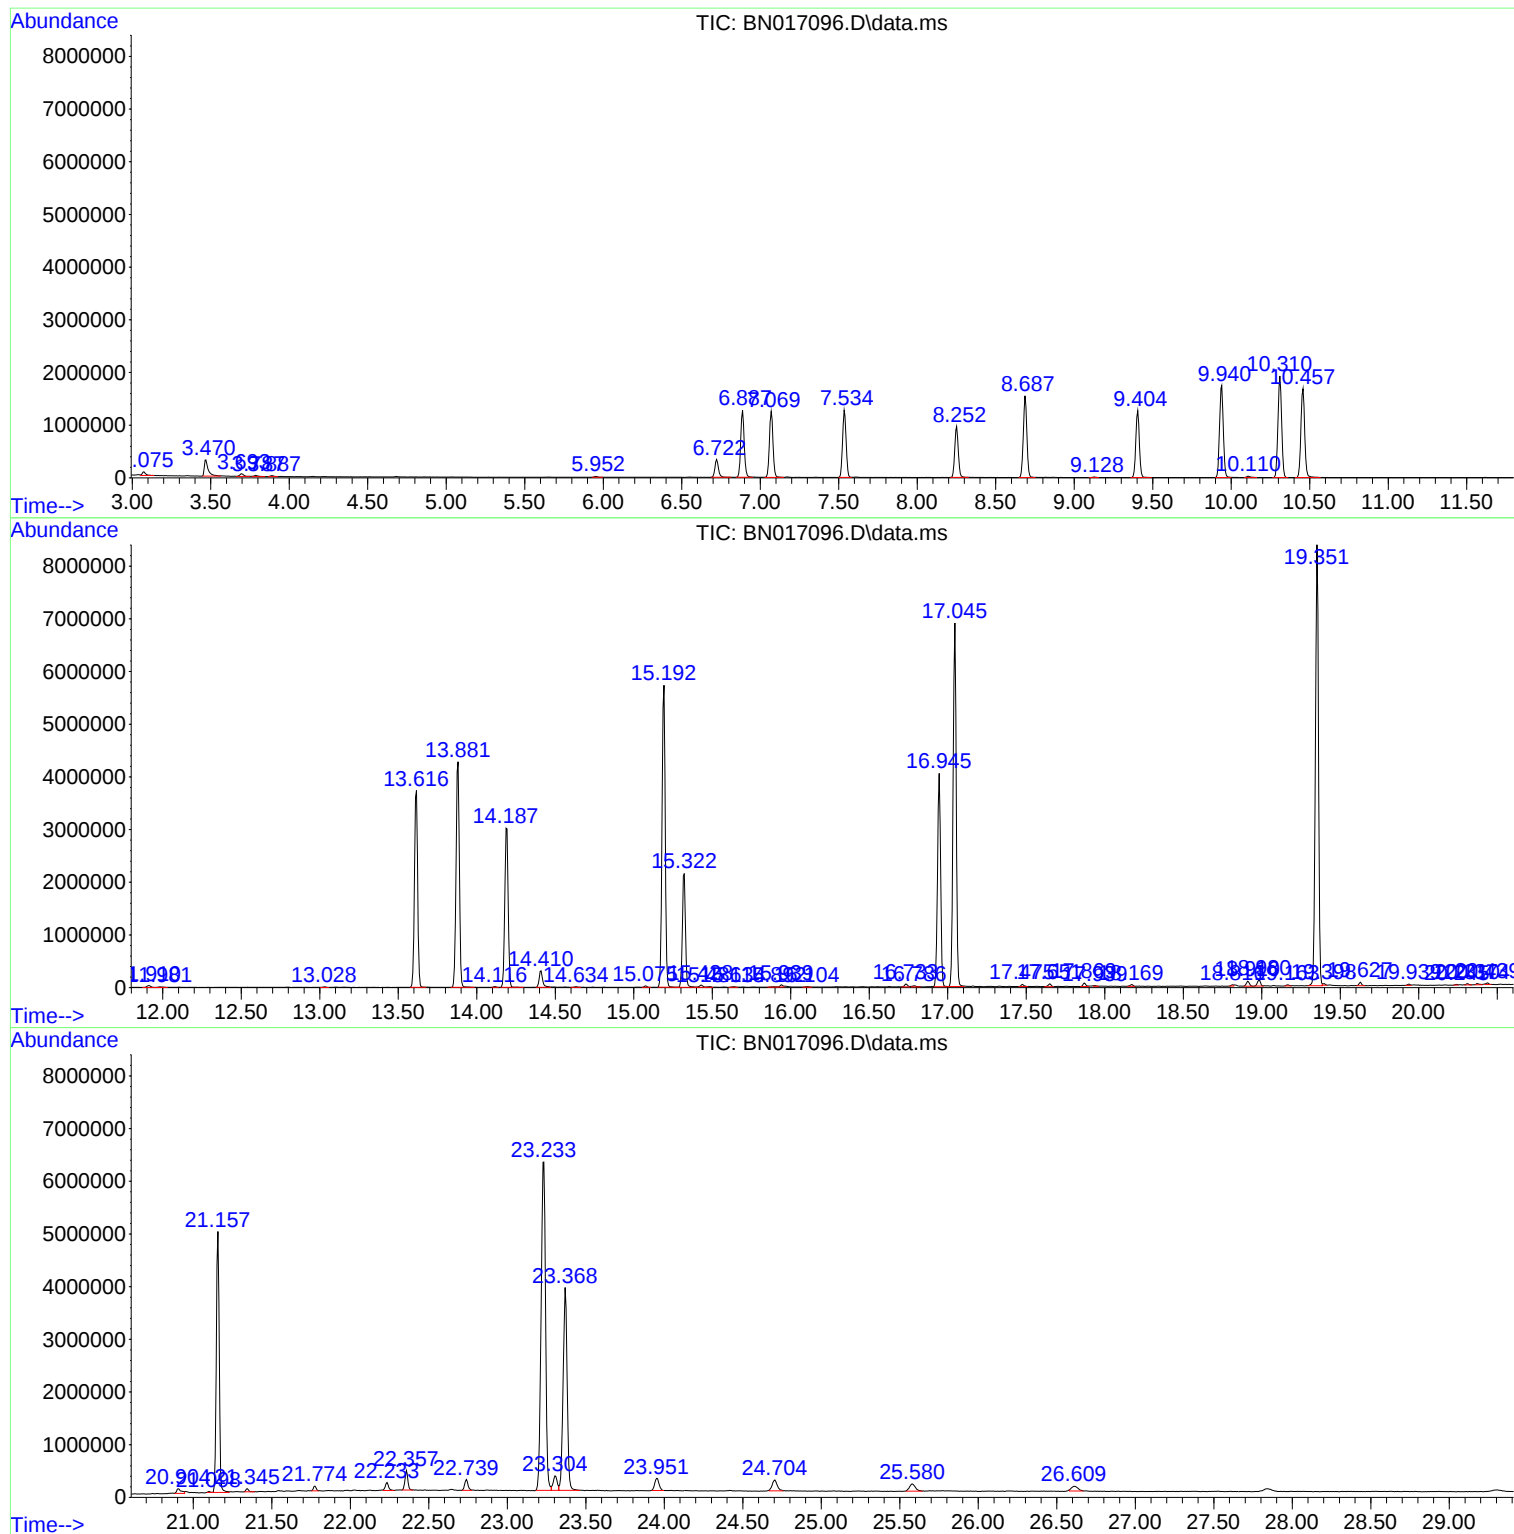

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102621\
Data File : BN017096.D
Acq On : 26 Oct 2021 18:14
Operator : CG/JU
Sample : M4318-08
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
P023-TW001-02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN102621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102621\
Data File : BN017096.D
Acq On : 26 Oct 2021 18:14
Operator : CG/JU
Sample : M4318-08
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
P023-TW001-02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN102621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------