

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102621\
 Data File : BN017099.D
 Acq On : 26 Oct 2021 20:04
 Operator : CG/JU
 Sample : M4319-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 P025-TW001-02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN102621.M
 Title : SVOA CALIBRATION

Signal : TIC: BN017099.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.070	10	14	22	rVB	59683	84513	0.86%	0.112%
2	3.470	79	82	91	rBV	50546	86728	0.89%	0.115%
3	3.693	115	120	127	rVB	33178	47908	0.49%	0.063%
4	3.787	132	136	142	rVB	15072	23657	0.24%	0.031%
5	3.887	150	153	157	rVB	11217	13341	0.14%	0.018%
6	4.687	284	289	294	rBV4	5644	11959	0.12%	0.016%
7	5.952	500	504	509	rVB3	10850	13993	0.14%	0.019%
8	6.722	629	635	643	rBV	205874	318532	3.25%	0.422%
9	6.887	655	663	676	rBV	806063	1261366	12.87%	1.672%
10	7.069	687	694	703	rBV	809232	1222145	12.47%	1.620%
11	7.175	708	712	716	rVB6	6627	10586	0.11%	0.014%
12	7.534	766	773	782	rBV	947684	1440433	14.70%	1.909%
13	7.763	808	812	820	rBV4	6716	11749	0.12%	0.016%
14	8.252	888	895	908	rVB	607676	961286	9.81%	1.274%
15	8.687	962	969	980	rBV	960879	1516596	15.48%	2.010%
16	9.405	1084	1091	1102	rBV	775091	1229891	12.55%	1.630%
17	9.940	1175	1182	1198	rBV	1092768	1796967	18.34%	2.381%
18	10.105	1204	1210	1224	rBV	171523	296176	3.02%	0.392%
19	10.310	1237	1245	1255	rVB	1423780	2285736	23.33%	3.029%
20	10.457	1263	1270	1280	rBV	579151	984510	10.05%	1.305%
21	11.910	1509	1517	1523	rBV	21728	36326	0.37%	0.048%
22	13.616	1800	1807	1820	rBV	2620065	3640887	37.16%	4.825%
23	13.875	1844	1851	1865	rBV	2849934	4159851	42.45%	5.513%
24	14.187	1898	1904	1913	rBV	2288969	3328799	33.97%	4.411%
25	14.410	1936	1942	1954	rBV	186687	318322	3.25%	0.422%
26	14.634	1976	1980	1985	rVB2	14606	17412	0.18%	0.023%
27	15.192	2068	2075	2090	rBV	3867398	5581548	56.96%	7.397%
28	15.316	2090	2096	2111	rVV	1496517	1997572	20.39%	2.647%
29	15.428	2111	2115	2120	rVB3	24863	31725	0.32%	0.042%
30	15.645	2149	2152	2156	rVB4	7896	10130	0.10%	0.013%
31	16.104	2226	2230	2237	rBB3	5755	10258	0.10%	0.014%
32	16.728	2330	2336	2341	rBV2	11968	17121	0.17%	0.023%
33	16.945	2366	2373	2383	rVB	2969464	4153805	42.39%	5.505%
34	17.045	2383	2390	2405	rBV	5075011	7147947	72.95%	9.472%
35	17.651	2487	2493	2499	rVB	86858	102094	1.04%	0.135%
36	17.869	2526	2530	2537	rBV2	35725	49164	0.50%	0.065%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102621\
 Data File : BN017099.D
 Acq On : 26 Oct 2021 20:04
 Operator : CG/JU
 Sample : M4319-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 P025-TW001-02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN102621.M
 Title : SVOA CALIBRATION

37	17.939	2537	2542	2547	rVB3	7566	11729	0.12%	0.016%
38	18.804	2685	2689	2690	rBV4	9806	11508	0.12%	0.015%
39	18.833	2690	2694	2699	rVV	97603	109727	1.12%	0.145%
40	18.916	2703	2708	2712	rVB	66975	87575	0.89%	0.116%
41	18.980	2712	2719	2724	rBV	72440	104043	1.06%	0.138%
42	19.163	2746	2750	2753	rBV4	9039	11310	0.12%	0.015%
43	19.351	2773	2782	2794	rBV	6498580	8697668	88.76%	11.526%
44	20.375	2952	2956	2959	rBV4	15058	21607	0.22%	0.029%
45	20.439	2963	2967	2970	rBV4	12244	16488	0.17%	0.022%
46	20.904	3041	3046	3051	rBV3	53214	99783	1.02%	0.132%
47	21.098	3077	3079	3083	rBV3	12881	14365	0.15%	0.019%
48	21.157	3083	3089	3102	rVV	4108707	5050460	51.54%	6.693%
49	21.339	3118	3120	3125	rVB2	23020	23024	0.23%	0.031%
50	21.774	3191	3194	3200	rBV	35203	43011	0.44%	0.057%
51	22.233	3269	3272	3280	rVB2	64183	95990	0.98%	0.127%
52	22.357	3288	3293	3298	rBV	154624	215345	2.20%	0.285%
53	22.739	3354	3358	3365	rVB	106439	146728	1.50%	0.194%
54	23.227	3433	3441	3450	rBV2	5376280	9798700	100.00%	12.985%
55	23.304	3450	3454	3458	rVV	169341	304674	3.11%	0.404%
56	23.369	3458	3465	3482	rVB2	3048819	5629812	57.45%	7.461%
57	23.951	3559	3564	3572	rVB	140257	263466	2.69%	0.349%
58	24.704	3686	3692	3701	rVB	130374	269804	2.75%	0.358%
59	25.580	3836	3841	3853	rVB2	84536	212840	2.17%	0.282%




Sum of corrected areas: 75460690

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102621\
Data File : BN017099.D
Acq On : 26 Oct 2021 20:04
Operator : CG/JU
Sample : M4319-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
P025-TW001-02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN102621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

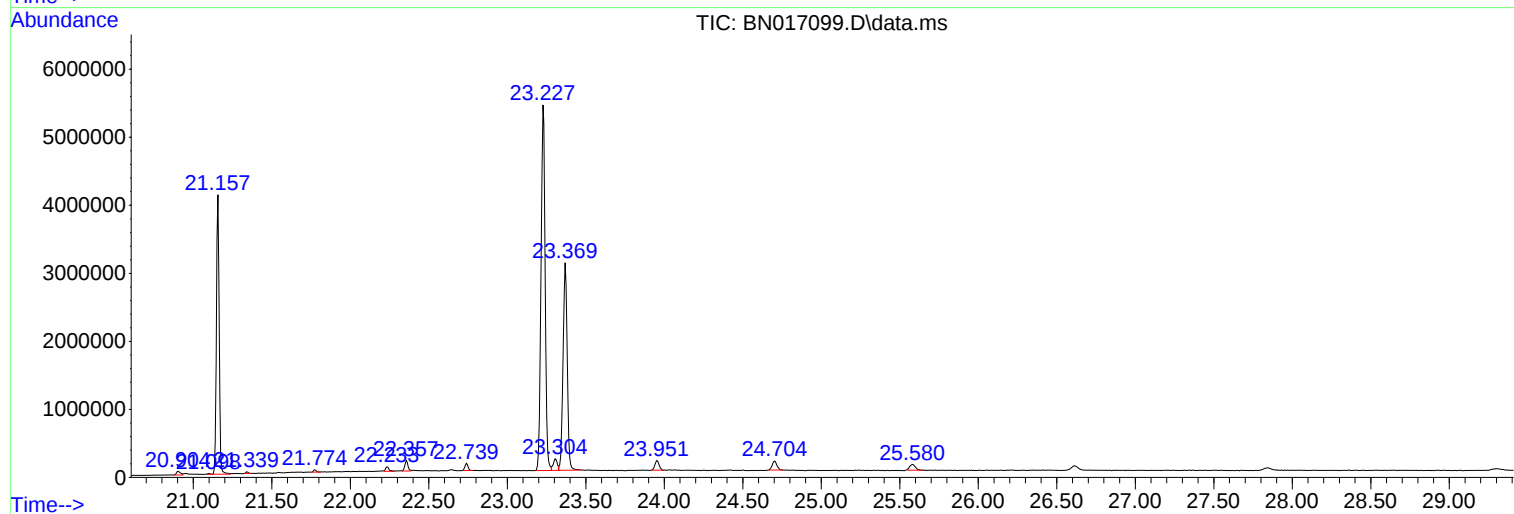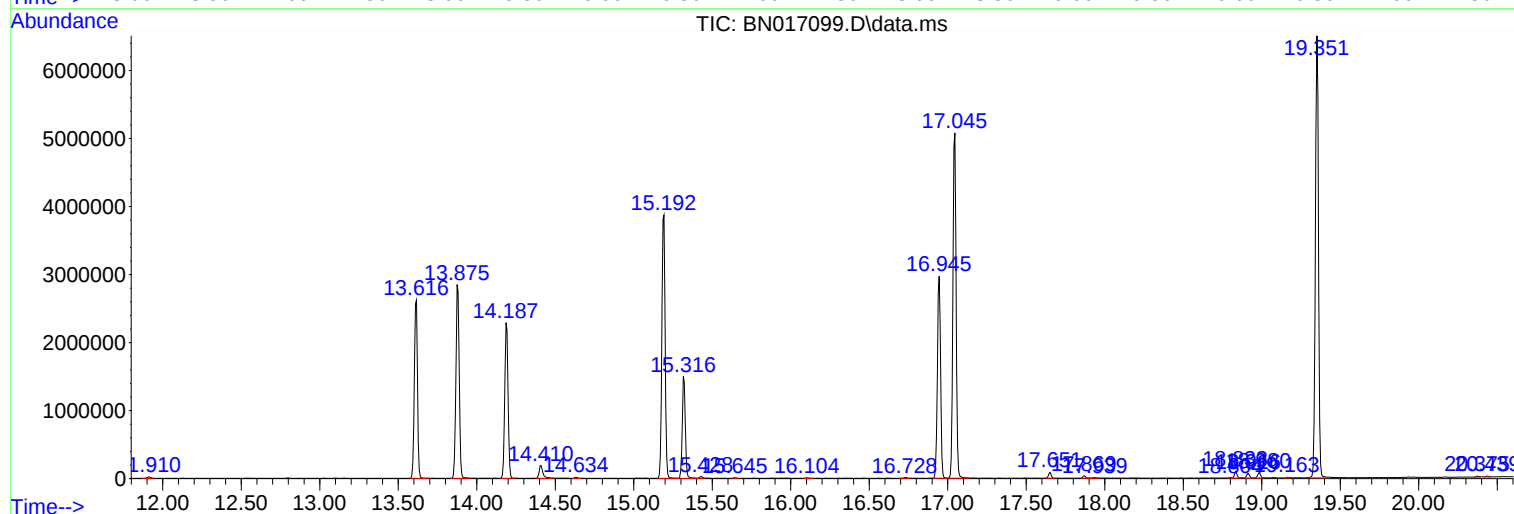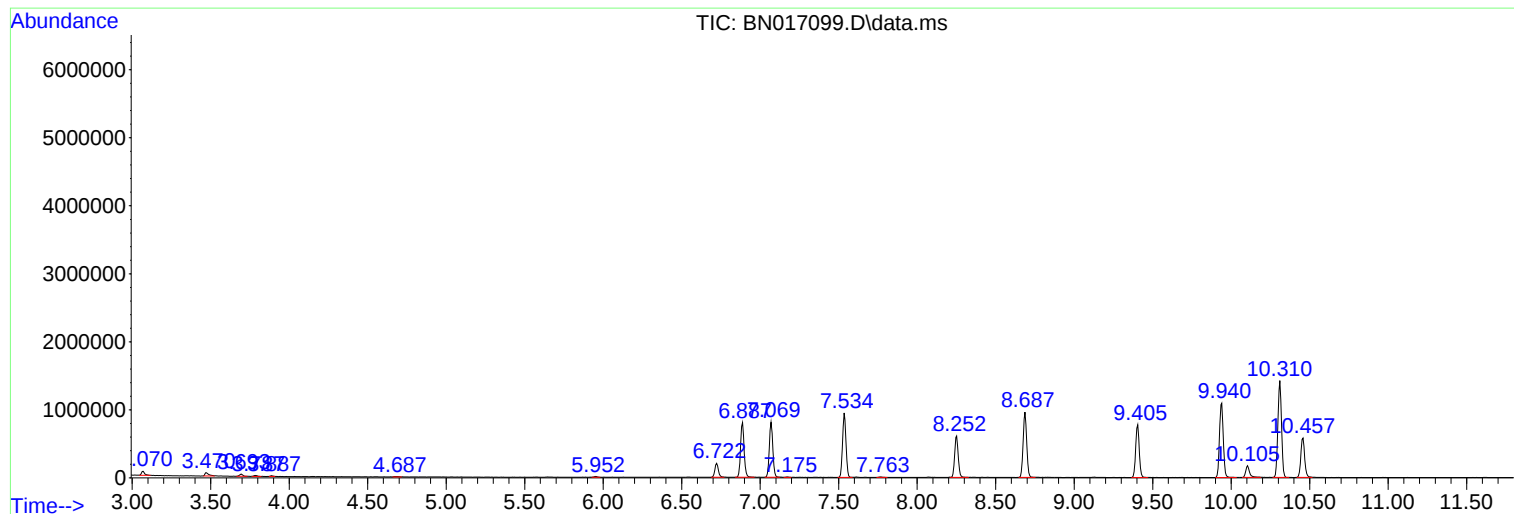

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102621\
Data File : BN017099.D
Acq On : 26 Oct 2021 20:04
Operator : CG/JU
Sample : M4319-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
P025-TW001-02










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN102621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethanol, 2-(2-butoxyethoxy)- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
10.105	2.59 ng/ul	296176	Naphthalene-d8	10.310

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
2			Ethanol, 1-(2-butoxyethoxy)-	162	C8H18O3	054446-78-5	90
3			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
4			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
5			Ethanol, 1-(2-butoxyethoxy)-	162	C8H18O3	054446-78-5	83

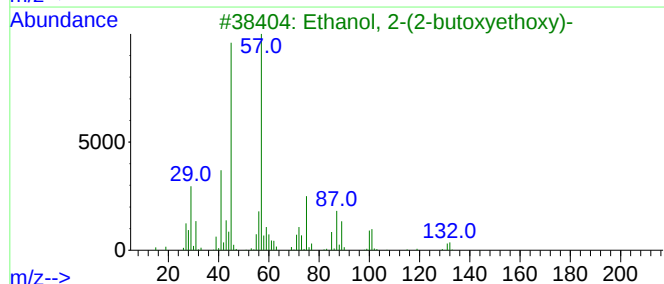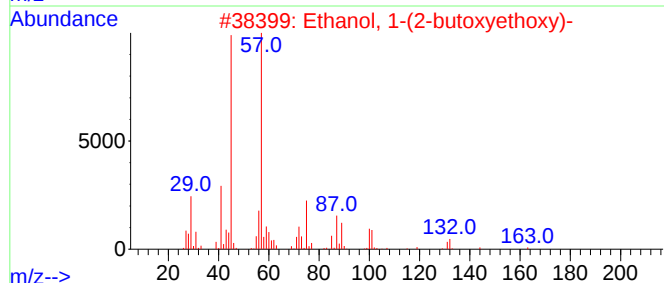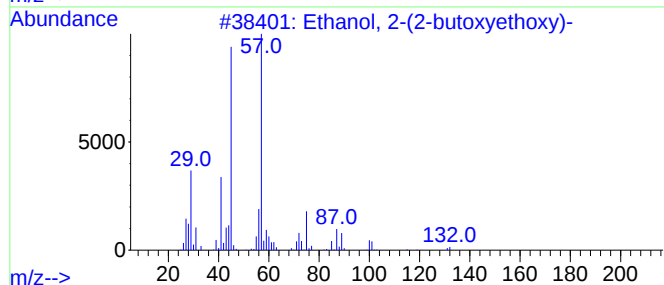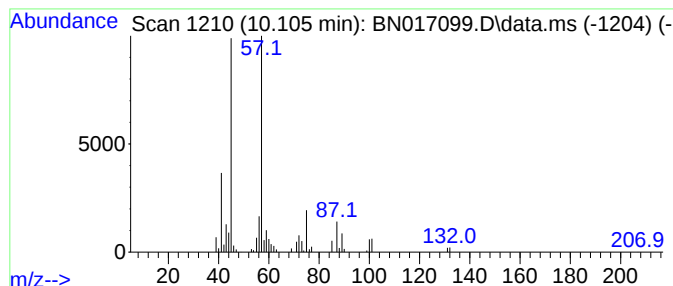

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102621\
Data File : BN017099.D
Acq On : 26 Oct 2021 20:04
Operator : CG/JU
Sample : M4319-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
P025-TW001-02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN102621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethanol, 2-(2-b...	10.105	2.6	ng/u1	296176	2	10.310	2285740	20.0