

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102621\
 Data File : BN017103.D
 Acq On : 26 Oct 2021 23:07
 Operator : CG/JU
 Sample : PB140249BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK249

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN102621.M
 Title : SVOA CALIBRATION

Signal : TIC: BN017103.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.070	10	14	22	rVB	63130	86188	1.05%	0.116%
2	3.458	76	80	108	rBV	837132	1312711	16.04%	1.761%
3	3.781	132	135	141	rVB	14648	19499	0.24%	0.026%
4	6.722	628	635	649	rBV	978673	1498282	18.30%	2.009%
5	6.887	656	663	677	rBV	793492	1258540	15.37%	1.688%
6	7.069	687	694	703	rBV	1008164	1551682	18.96%	2.081%
7	7.534	767	773	783	rBV	856157	1312357	16.03%	1.760%
8	8.252	888	895	907	rBV	1230511	1931656	23.60%	2.591%
9	8.687	961	969	978	rBV	965759	1521964	18.59%	2.041%
10	9.405	1084	1091	1105	rVB	782986	1276287	15.59%	1.712%
11	9.934	1175	1181	1197	rBV	1194520	1936372	23.65%	2.597%
12	10.310	1235	1245	1253	rBV	1307776	2122964	25.93%	2.847%
13	10.458	1262	1270	1286	rBV	1288263	2217357	27.09%	2.974%
14	11.910	1512	1517	1527	rBV	19258	32636	0.40%	0.044%
15	13.610	1800	1806	1817	rBV	2585554	3528328	43.10%	4.732%
16	13.875	1845	1851	1867	rBV	2813393	4086447	49.92%	5.480%
17	14.187	1897	1904	1912	rBV	2193478	3150337	38.48%	4.225%
18	14.410	1935	1942	1960	rBV	1113493	1627947	19.89%	2.183%
19	15.187	2068	2074	2086	rBV	3680226	5227295	63.86%	7.010%
20	15.316	2090	2096	2111	rVV	1314290	1704499	20.82%	2.286%
21	15.428	2111	2115	2123	rVB	21441	30921	0.38%	0.041%
22	16.734	2331	2337	2342	rBV	8818	13102	0.16%	0.018%
23	16.945	2366	2373	2383	rBV	2870474	3944307	48.18%	5.290%
24	17.040	2383	2389	2407	rVV2	4256271	6099114	74.51%	8.180%
25	18.916	2702	2708	2712	rBV	44637	61246	0.75%	0.082%
26	18.986	2714	2720	2728	rVV	48166	67068	0.82%	0.090%
27	19.351	2773	2782	2795	rBV	5422362	7335596	89.61%	9.838%
28	20.375	2953	2956	2958	rBV3	6205	8317	0.10%	0.011%
29	21.151	3083	3088	3100	rBV	3504178	4556830	55.67%	6.111%
30	21.769	3190	3193	3199	rVB3	24170	30968	0.38%	0.042%
31	22.233	3268	3272	3276	rVB	58951	78905	0.96%	0.106%
32	22.733	3353	3357	3364	rVB	100442	152632	1.86%	0.205%
33	23.222	3432	3440	3449	rBV	4647533	8186070	100.00%	10.979%
34	23.298	3449	3453	3457	rVV	175778	311223	3.80%	0.417%
35	23.363	3457	3464	3477	rVB2	2735051	5017868	61.30%	6.730%
36	23.951	3558	3564	3574	rVB	174098	330448	4.04%	0.443%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102621\
Data File : BN017103.D
Acq On : 26 Oct 2021 23:07
Operator : CG/JU
Sample : PB140249BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK249

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN102621.M
Title : SVOA CALIBRATION

37	24.698	3685	3691	3700	rVB	167780	349482	4.27%	0.469%
38	25.574	3834	3840	3854	rVB2	125758	315635	3.86%	0.423%
39	26.610	4009	4016	4026	rVB3	95554	270896	3.31%	0.363%


Sum of corrected areas: 74563976

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102621\
Data File : BN017103.D
Acq On : 26 Oct 2021 23:07
Operator : CG/JU
Sample : PB140249BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK249

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN102621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

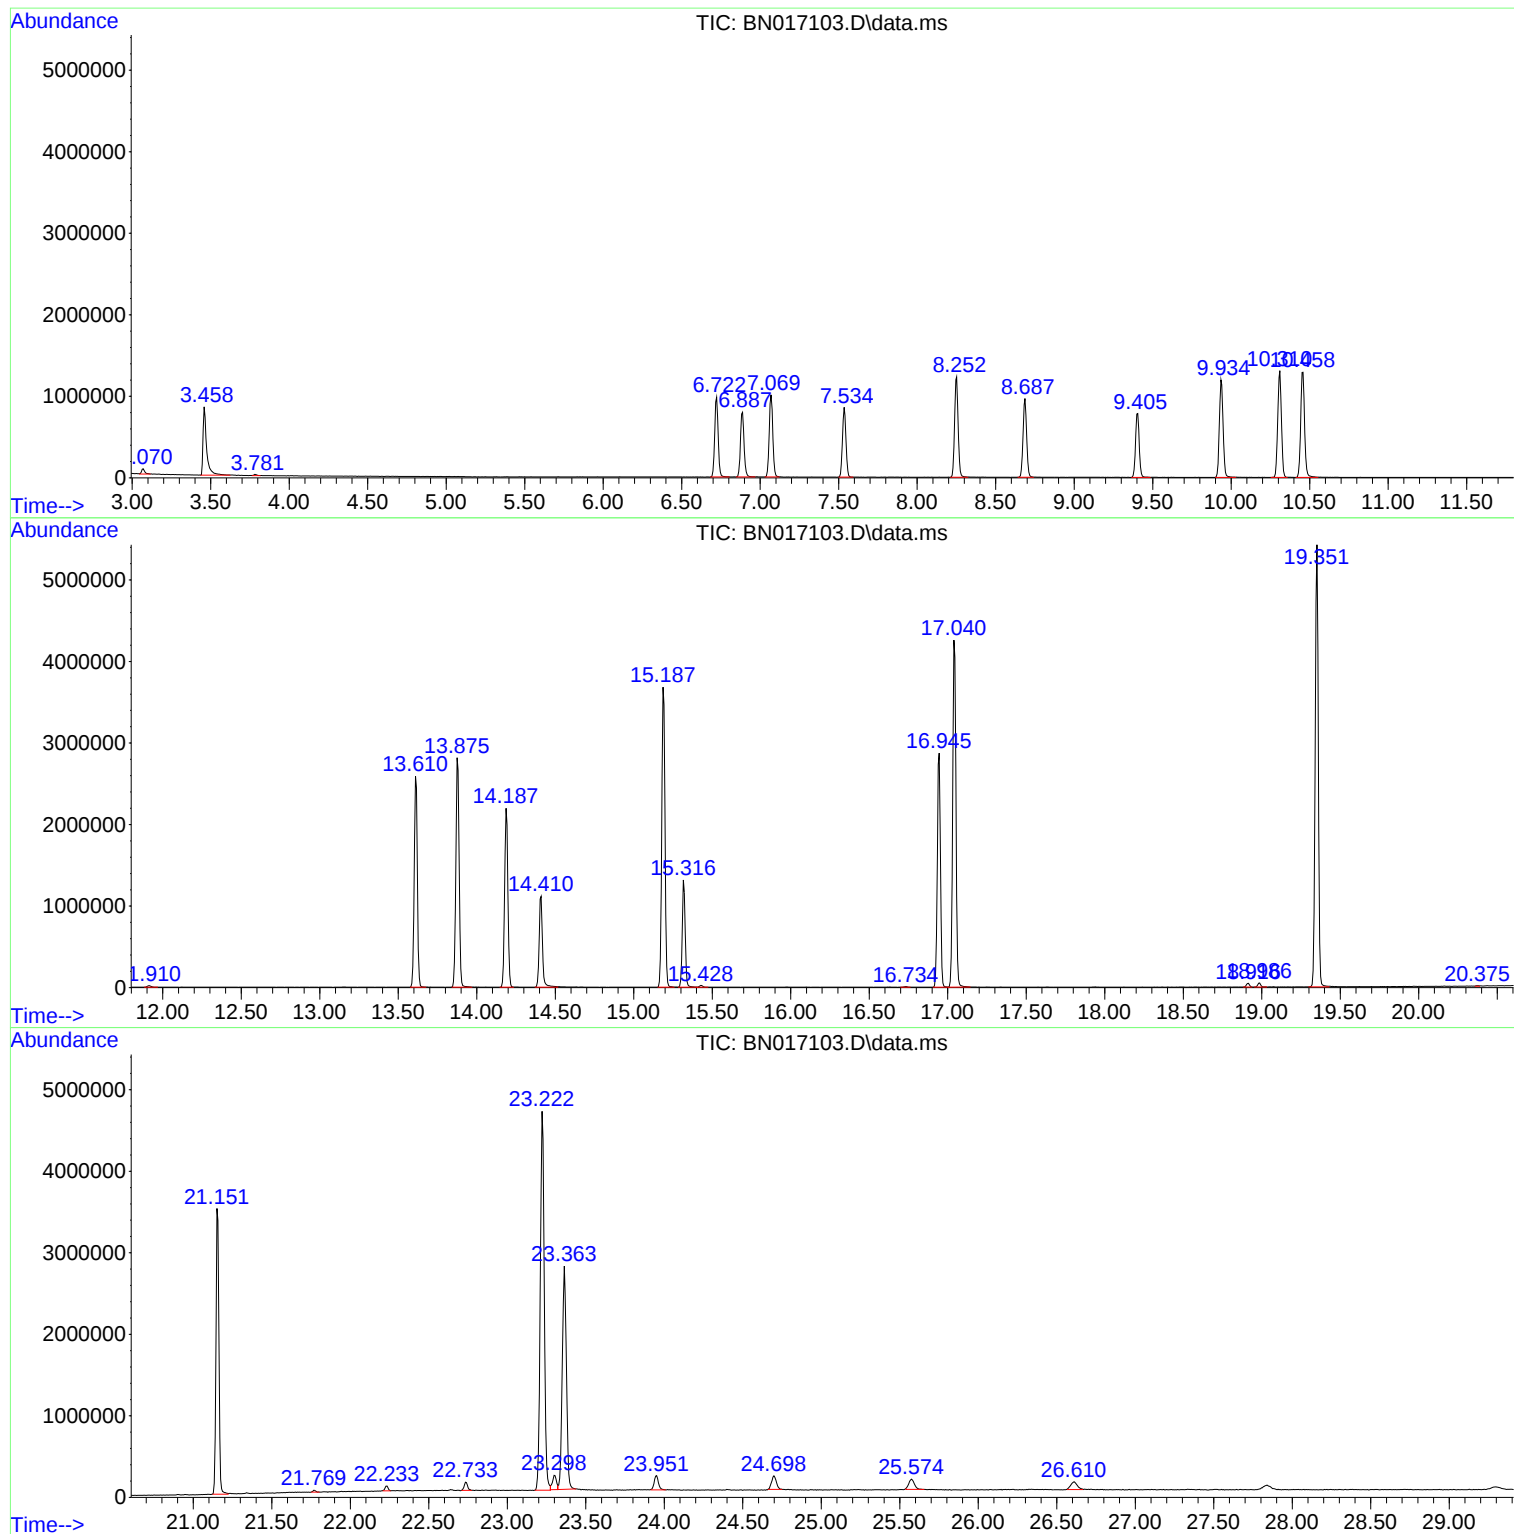

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102621\
Data File : BN017103.D
Acq On : 26 Oct 2021 23:07
Operator : CG/JU
Sample : PB140249BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK249

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN102621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102621\
Data File : BN017103.D
Acq On : 26 Oct 2021 23:07
Operator : CG/JU
Sample : PB140249BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK249

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN102621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
