

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102621\
 Data File : BN017112.D
 Acq On : 27 Oct 2021 04:34
 Operator : CG/JU
 Sample : M4319-11
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 P071-TW001-01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN102621.M
 Title : SVOA CALIBRATION

Signal : TIC: BN017112.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.069	10	14	23	rVB	73475	108528	0.85%	0.102%
2	3.464	77	81	99	rBV	337658	554978	4.33%	0.522%
3	3.693	115	120	126	rVB	51811	77619	0.61%	0.073%
4	3.781	132	135	146	rVV2	20914	34359	0.27%	0.032%
5	3.887	149	153	159	rVB4	19109	28041	0.22%	0.026%
6	4.675	285	287	298	rVB5	10959	21030	0.16%	0.020%
7	5.952	500	504	513	rVB2	16691	25821	0.20%	0.024%
8	6.546	601	605	612	rBV3	9052	19862	0.16%	0.019%
9	6.722	629	635	642	rBV	331945	510726	3.99%	0.481%
10	6.887	656	663	678	rBV	1170674	1870108	14.60%	1.760%
11	7.069	687	694	705	rBV	1201245	1836554	14.34%	1.728%
12	7.169	706	711	719	rVB8	10122	18718	0.15%	0.018%
13	7.534	766	773	782	rBV	1184268	1818955	14.20%	1.712%
14	7.763	808	812	822	rVB6	10598	17849	0.14%	0.017%
15	8.246	888	894	911	rVB	960646	1534039	11.98%	1.444%
16	8.687	961	969	980	rBV	1460104	2310700	18.04%	2.175%
17	8.863	996	999	1006	rVB3	12758	17219	0.13%	0.016%
18	9.404	1084	1091	1104	rBV	1158223	1891737	14.77%	1.780%
19	9.934	1174	1181	1197	rBV	1703454	2752750	21.49%	2.591%
20	10.104	1203	1210	1229	rBV	423714	688816	5.38%	0.648%
21	10.310	1237	1245	1253	rBV	1787076	2987731	23.32%	2.812%
22	10.451	1261	1269	1290	rBV	1579553	2759700	21.54%	2.597%
23	11.128	1379	1384	1390	rBV5	5567	13099	0.10%	0.012%
24	11.910	1510	1517	1522	rBV2	33256	55663	0.43%	0.052%
25	11.987	1524	1530	1541	rBV3	15574	39245	0.31%	0.037%
26	12.792	1664	1667	1672	rBV2	15455	21430	0.17%	0.020%
27	13.098	1712	1719	1725	rBV	52657	77948	0.61%	0.073%
28	13.610	1800	1806	1818	rBV	3651226	5107126	39.87%	4.807%
29	13.875	1844	1851	1866	rBV	4145867	6150480	48.01%	5.789%
30	14.187	1897	1904	1912	rBV	3020624	4304868	33.61%	4.052%
31	14.404	1936	1941	1957	rBV	341419	531494	4.15%	0.500%
32	14.634	1976	1980	1986	rBV4	15504	20151	0.16%	0.019%
33	15.016	2039	2045	2046	rBV	10944	14355	0.11%	0.014%
34	15.186	2067	2074	2090	rBV	5318985	7765680	60.62%	7.309%
35	15.316	2090	2096	2110	rVV	2152062	2822112	22.03%	2.656%
36	15.428	2110	2115	2120	rVB	41685	55406	0.43%	0.052%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102621\
 Data File : BN017112.D
 Acq On : 27 Oct 2021 04:34
 Operator : CG/JU
 Sample : M4319-11
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 P071-TW001-01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN102621.M
 Title : SVOA CALIBRATION

37	15.645	2148	2152	2158	rVB3	12909	18829	0.15%	0.018%
38	16.104	2223	2230	2234	rBV3	11439	20855	0.16%	0.020%
39	16.728	2332	2336	2341	rBV2	19218	26314	0.21%	0.025%
40	16.945	2366	2373	2383	rBV	3774407	5307251	41.43%	4.995%
41	17.045	2383	2390	2405	rBV	6674619	9638806	75.24%	9.072%
42	17.157	2405	2409	2414	rVB	32697	43716	0.34%	0.041%
43	17.651	2487	2493	2499	rVB	162047	200138	1.56%	0.188%
44	17.869	2525	2530	2537	rBV	100492	143922	1.12%	0.135%
45	17.933	2538	2541	2546	rVB	20716	28368	0.22%	0.027%
46	18.804	2683	2689	2690	rBV3	16489	23924	0.19%	0.023%
47	18.833	2690	2694	2698	rVV	194307	231601	1.81%	0.218%
48	18.910	2702	2707	2712	rVB2	94324	127399	0.99%	0.120%
49	18.975	2712	2718	2724	rBV2	163400	262230	2.05%	0.247%
50	19.069	2732	2734	2742	rVB5	10670	15934	0.12%	0.015%
51	19.163	2747	2750	2755	rBV3	37180	49559	0.39%	0.047%
52	19.351	2771	2782	2788	rBV	8414369	11449528	89.38%	10.776%
53	19.427	2794	2795	2800	rVB4	11981	13502	0.11%	0.013%
54	19.933	2878	2881	2884	rBV3	13013	15113	0.12%	0.014%
55	19.998	2890	2892	2898	rVB5	15927	20228	0.16%	0.019%
56	20.080	2902	2906	2909	rVB4	11820	13342	0.10%	0.013%
57	20.310	2941	2945	2951	rBV	68401	72976	0.57%	0.069%
58	20.369	2952	2955	2961	rVV3	22267	31979	0.25%	0.030%
59	20.433	2961	2966	2970	rVV2	24381	35079	0.27%	0.033%
60	20.904	3041	3046	3053	rBV	77889	164150	1.28%	0.154%
61	21.098	3076	3079	3083	rBV	21765	21901	0.17%	0.021%
62	21.151	3083	3088	3099	rBV	4738913	6317496	49.32%	5.946%
63	21.339	3117	3120	3123	rBV2	42534	43405	0.34%	0.041%
64	21.768	3190	3193	3200	rBV	59199	73692	0.58%	0.069%
65	22.221	3265	3270	3281	rBV2	324421	564125	4.40%	0.531%
66	22.357	3288	3293	3298	rBV	168755	231859	1.81%	0.218%
67	22.733	3353	3357	3368	rVB	177257	269693	2.11%	0.254%
68	23.227	3432	3441	3449	rBV	6787561	12810115	100.00%	12.056%
69	23.304	3449	3454	3458	rVV	270780	497910	3.89%	0.469%
70	23.368	3458	3465	3480	rVB2	3827775	6960157	54.33%	6.551%
71	23.951	3558	3564	3573	rVB	242476	462876	3.61%	0.436%
72	24.698	3684	3691	3705	rVB2	209070	496335	3.87%	0.467%
73	25.574	3833	3840	3856	rVB2	141609	387912	3.03%	0.365%
74	26.604	4010	4015	4029	rVB6	96668	295748	2.31%	0.278%

Sum of corrected areas: 106252864

Instrument :

BNA_N

ClientSampleId :


P071-TW001-01

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102621\
Data File : BN017112.D
Acq On : 27 Oct 2021 04:34
Operator : CG/JU
Sample : M4319-11
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
P071-TW001-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN102621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

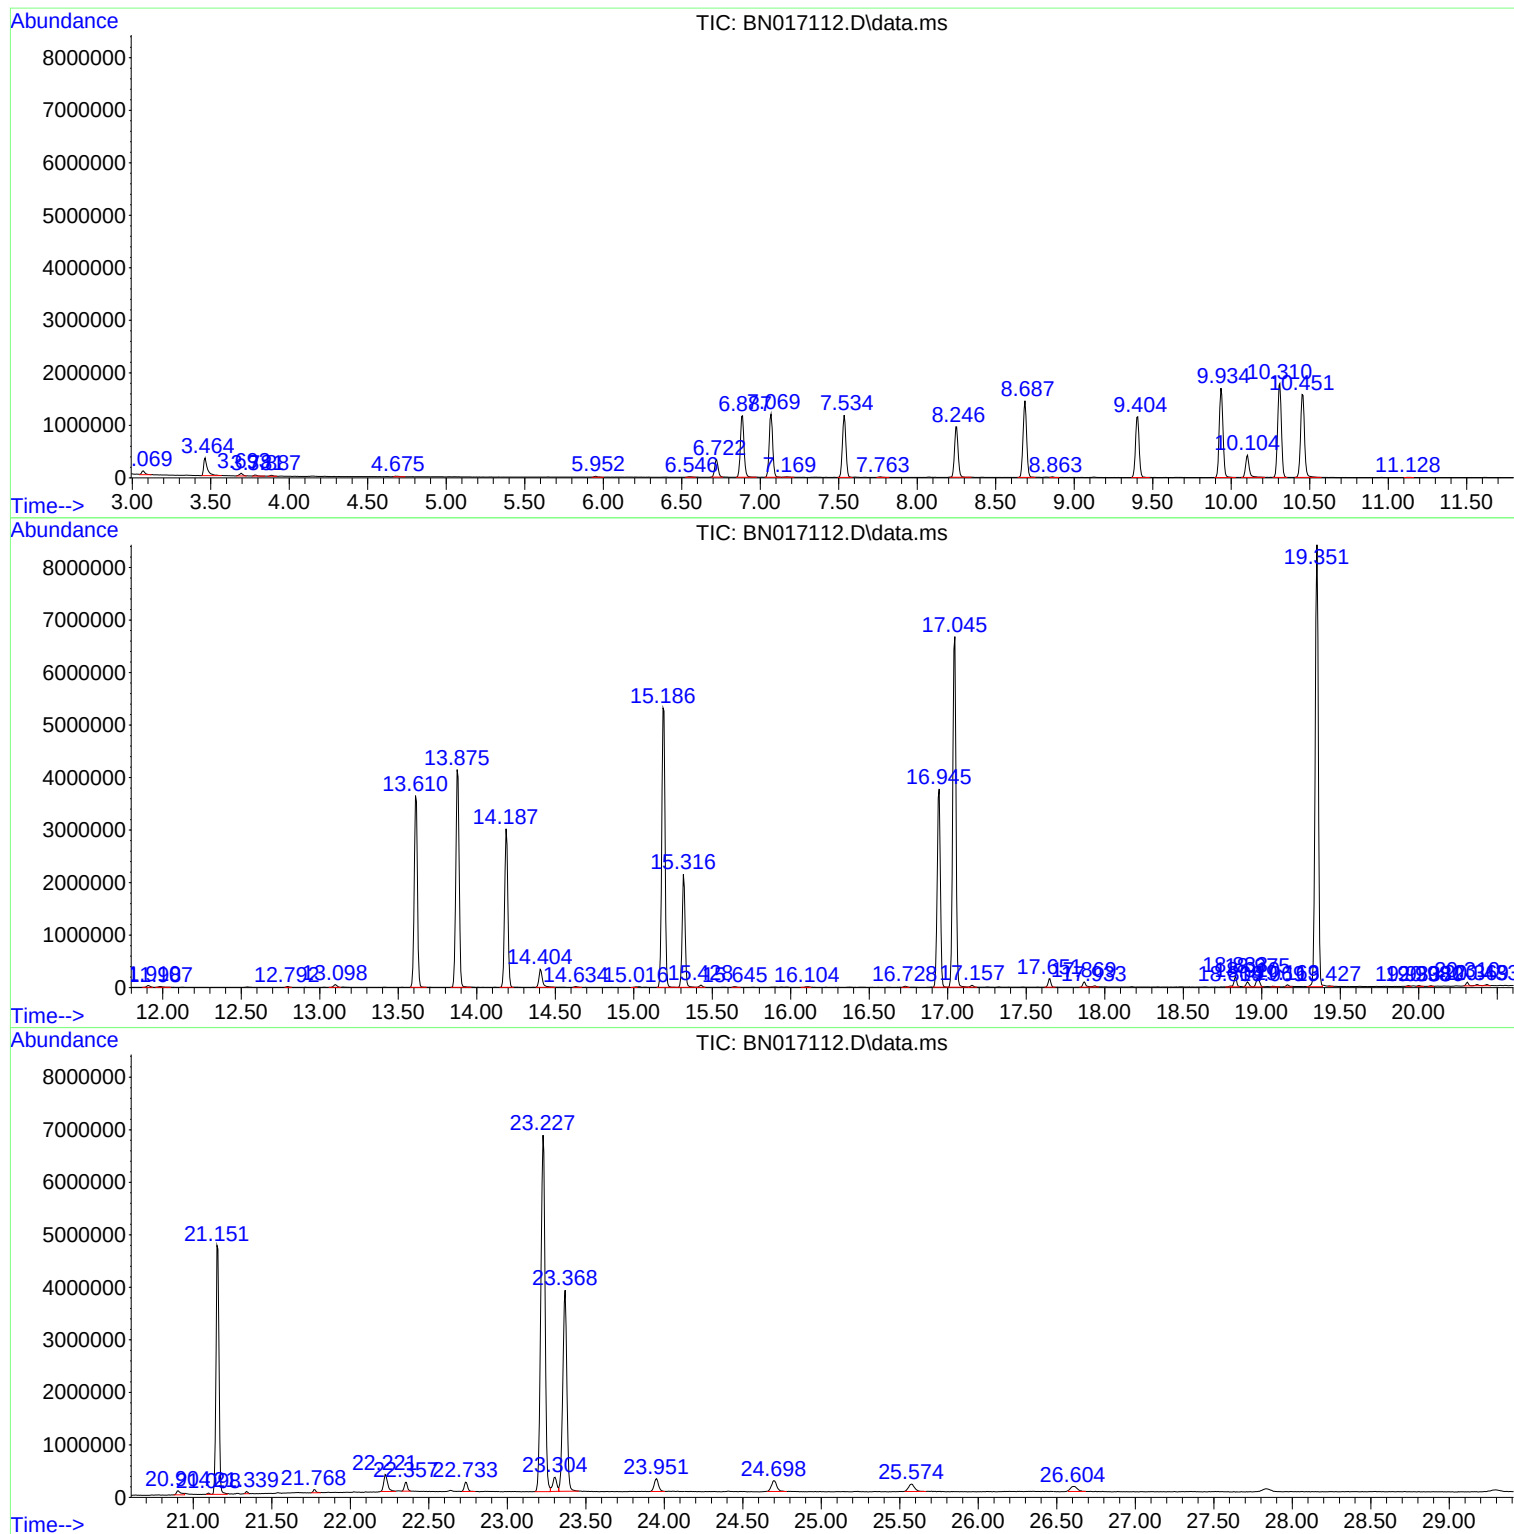

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102621\
Data File : BN017112.D
Acq On : 27 Oct 2021 04:34
Operator : CG/JU
Sample : M4319-11
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
P071-TW001-01










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN102621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethanol, 2-(2-butoxyethoxy)- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
10.104	4.61 ng/ul	688816	Naphthalene-d8	10.310

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
2			Ethanol, 1-(2-butoxyethoxy)-	162	C8H18O3	054446-78-5	90
3			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	86
4			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	83
5			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	78

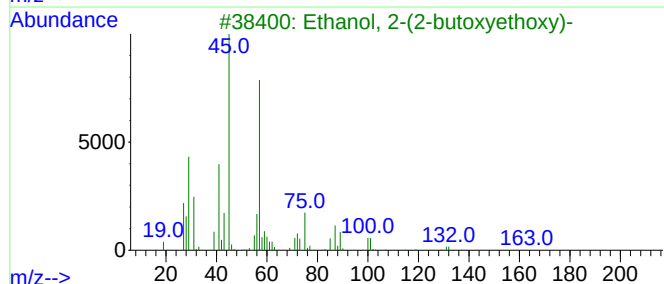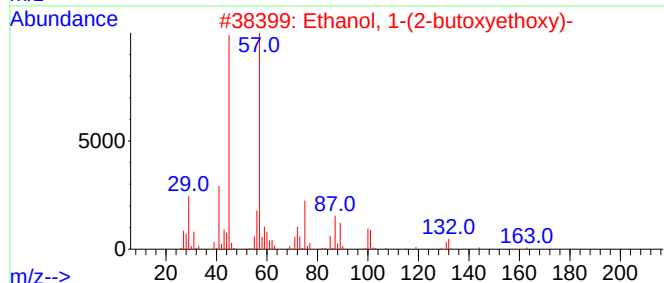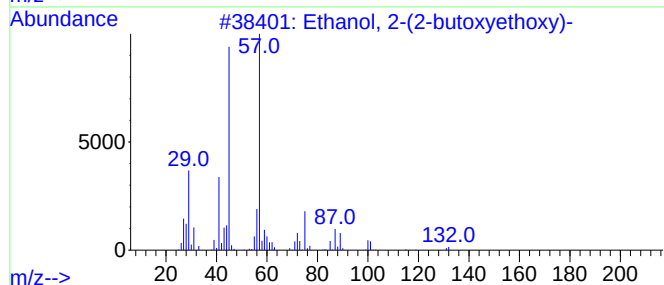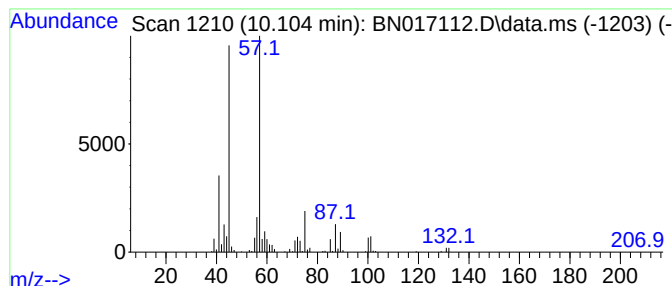

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102621\
Data File : BN017112.D
Acq On : 27 Oct 2021 04:34
Operator : CG/JU
Sample : M4319-11
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
P071-TW001-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN102621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethanol, 2-(2-b...	10.104	4.6	ng/u1	688816	2	10.310	2987730	20.0