

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102621\
 Data File : BN017118.D
 Acq On : 27 Oct 2021 08:48
 Operator : CG/JU
 Sample : PB140099BL
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK099

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN102621.M
 Title : SVOA CALIBRATION

Signal : TIC: BN017118.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.069	10	14	26	rVB	61744	96637	1.10%	0.117%
2	3.458	76	80	102	rBV	802779	1255011	14.27%	1.517%
3	3.787	132	136	141	rVB2	13297	18563	0.21%	0.022%
4	6.722	628	635	652	rBV	1005863	1557171	17.70%	1.882%
5	6.887	656	663	675	rBV	796123	1273995	14.48%	1.540%
6	7.069	687	694	707	rVB	1035070	1613046	18.34%	1.949%
7	7.534	766	773	781	rBV	966368	1497250	17.02%	1.809%
8	8.252	888	895	906	rBV	1293976	2048995	23.29%	2.476%
9	8.687	960	969	981	rBV	984928	1595745	18.14%	1.928%
10	9.399	1083	1090	1098	rBV	851286	1365588	15.52%	1.650%
11	9.934	1174	1181	1192	rBV	1266404	2052631	23.34%	2.480%
12	10.310	1237	1245	1253	rBV	1464662	2464668	28.02%	2.978%
13	10.451	1262	1269	1285	rBV	1368829	2316022	26.33%	2.799%
14	11.910	1511	1517	1523	rBV	20887	32782	0.37%	0.040%
15	13.610	1800	1806	1818	rBV	2821780	3871067	44.01%	4.678%
16	13.875	1844	1851	1867	rBV	3121249	4361117	49.58%	5.270%
17	14.186	1897	1904	1912	rBV	2576166	3668065	41.70%	4.433%
18	14.410	1935	1942	1964	rBV	1302592	1934648	21.99%	2.338%
19	15.186	2067	2074	2090	rBV	3996268	5659455	64.34%	6.839%
20	15.316	2090	2096	2109	rVV	1511570	1962162	22.31%	2.371%
21	15.428	2111	2115	2124	rVB2	44511	63003	0.72%	0.076%
22	16.728	2332	2336	2340	rBV4	11089	14552	0.17%	0.018%
23	16.945	2366	2373	2383	rVB	3210138	4559443	51.83%	5.510%
24	17.039	2383	2389	2404	rBV	4693461	6643344	75.53%	8.028%
25	18.910	2703	2707	2712	rVB	54542	69705	0.79%	0.084%
26	18.980	2714	2719	2724	rBV	56432	76031	0.86%	0.092%
27	19.351	2773	2782	2795	rBV	5998101	7915876	89.99%	9.566%
28	20.374	2952	2956	2957	rBV3	8104	9800	0.11%	0.012%
29	20.904	3043	3046	3050	rBV4	12016	15253	0.17%	0.018%
30	21.157	3083	3089	3102	rBV	4223929	5471936	62.21%	6.612%
31	21.339	3118	3120	3124	rBV2	18774	17649	0.20%	0.021%
32	21.774	3191	3194	3197	rVB	36888	36281	0.41%	0.044%
33	22.233	3268	3272	3277	rVB	93259	117955	1.34%	0.143%
34	22.733	3353	3357	3363	rVB	144845	209221	2.38%	0.253%
35	23.227	3433	3441	3449	rBV2	4796350	8796152	100.00%	10.630%
36	23.304	3450	3454	3458	rVV	232478	400096	4.55%	0.483%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102621\
Data File : BN017118.D
Acq On : 27 Oct 2021 08:48
Operator : CG/JU
Sample : PB140099BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK099

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN102621.M
Title : SVOA CALIBRATION

37	23.368	3458	3465	3482	rVB2	3188283	5917214	67.27%	7.151%
38	23.951	3558	3564	3575	rVB	235052	468874	5.33%	0.567%
39	24.698	3684	3691	3699	rVB2	225898	515324	5.86%	0.623%
40	25.574	3833	3840	3854	rVB2	166347	438403	4.98%	0.530%
41	26.609	4010	4016	4027	rVB3	120887	351267	3.99%	0.424%


Sum of corrected areas: 82751997

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102621\
Data File : BN017118.D
Acq On : 27 Oct 2021 08:48
Operator : CG/JU
Sample : PB140099BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK099

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN102621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

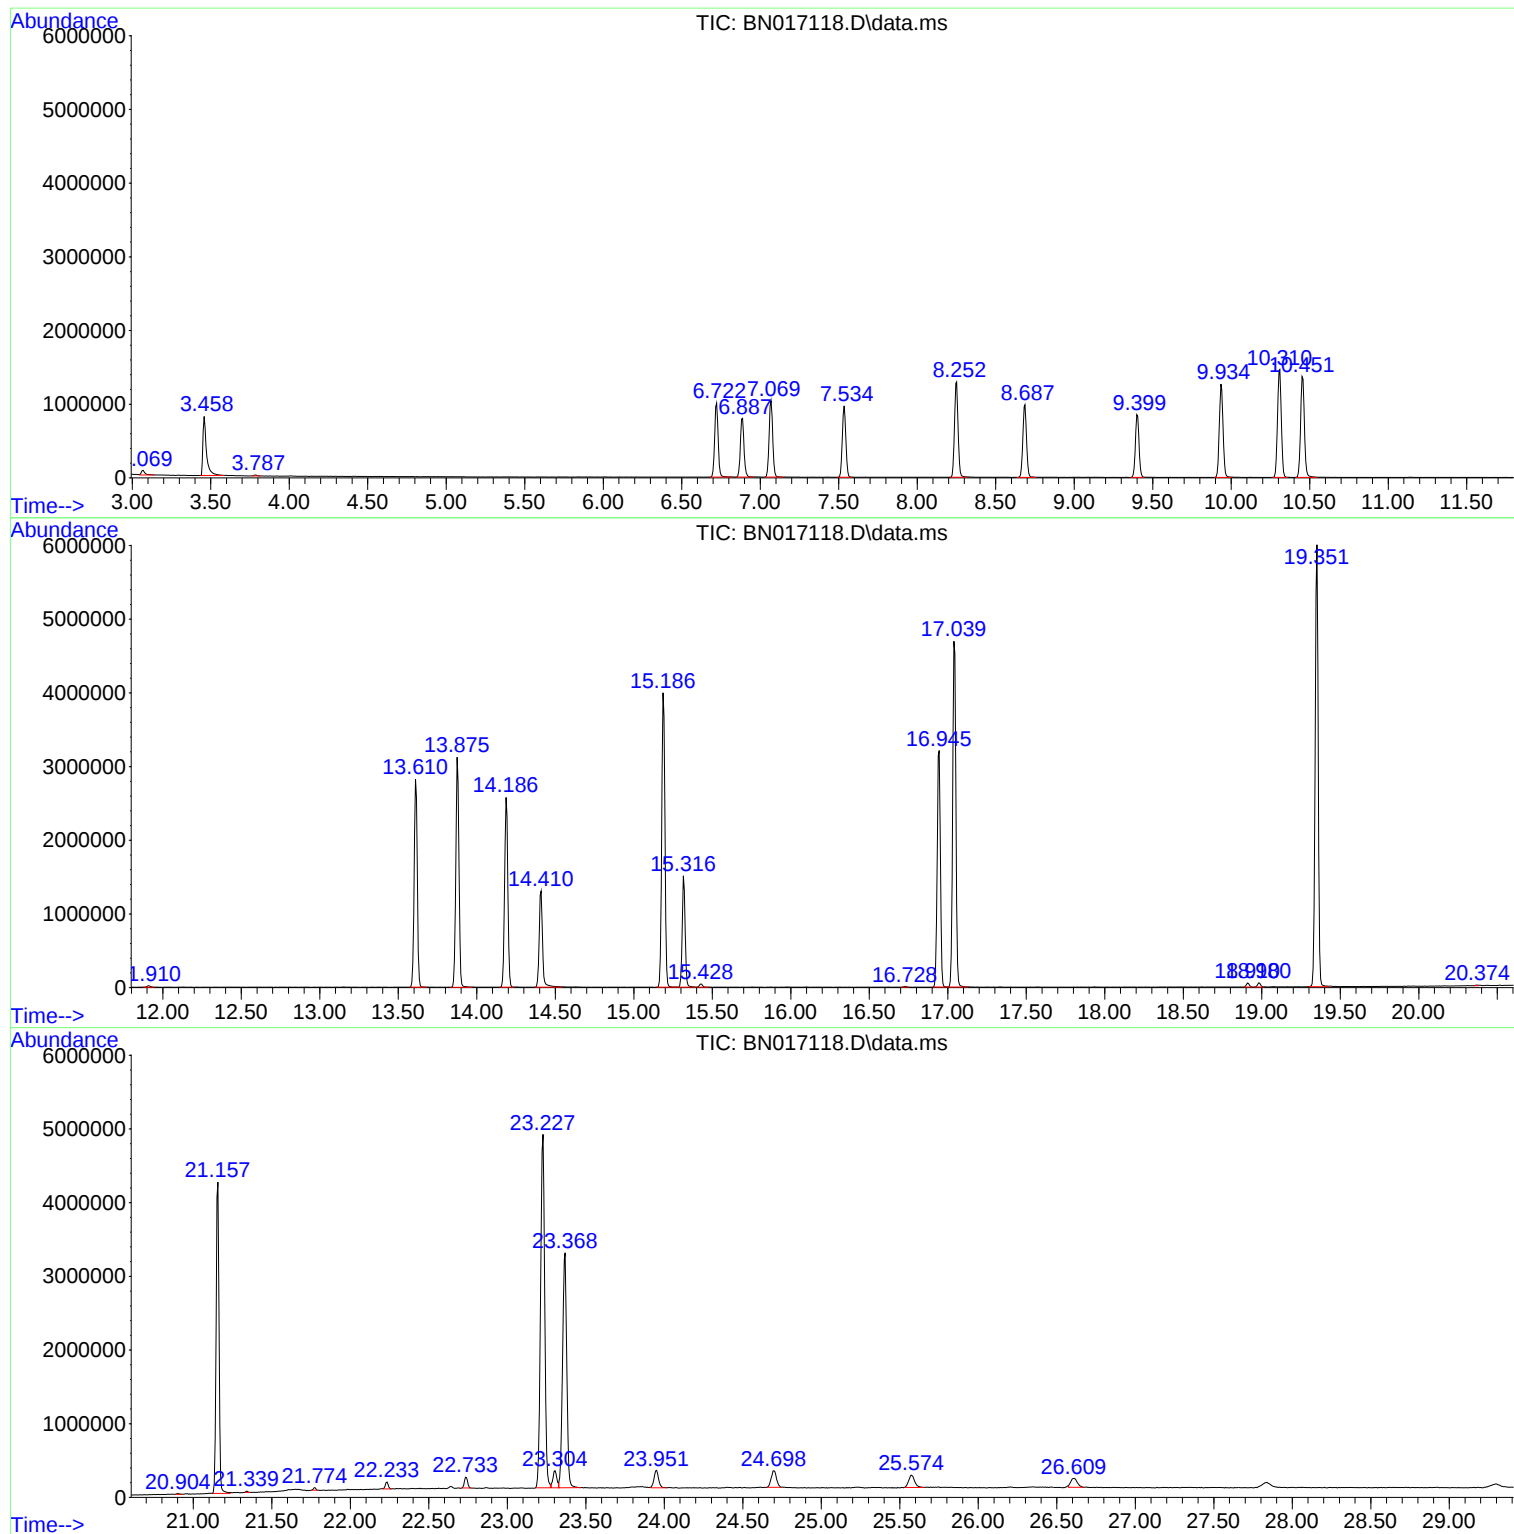

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102621\
Data File : BN017118.D
Acq On : 27 Oct 2021 08:48
Operator : CG/JU
Sample : PB140099BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK099

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN102621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102621\
Data File : BN017118.D
Acq On : 27 Oct 2021 08:48
Operator : CG/JU
Sample : PB140099BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK099

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN102621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
