

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102621\
 Data File : BN017121.D
 Acq On : 27 Oct 2021 10:37
 Operator : CG/JU
 Sample : M4215-10
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JDGC9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN102621.M
 Title : SVOA CALIBRATION

Signal : TIC: BN017121.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.575	98	100	105	rVB4	10724	12443	0.18%	0.029%
2	3.693	115	120	128	rVV	66362	101852	1.49%	0.239%
3	3.787	132	136	142	rVB	21528	31438	0.46%	0.074%
4	3.887	149	153	160	rVB4	26110	39921	0.58%	0.094%
5	4.146	195	197	205	rVB5	11208	17055	0.25%	0.040%
6	4.228	209	211	216	rVV3	7286	7514	0.11%	0.018%
7	4.675	282	287	298	rVB2	38719	72094	1.05%	0.169%
8	5.075	352	355	360	rVB	9771	14488	0.21%	0.034%
9	5.952	500	504	512	rVB	26366	37633	0.55%	0.088%
10	6.722	624	635	644	rBV	190332	313901	4.58%	0.737%
11	6.887	657	663	672	rBV	168530	272195	3.97%	0.639%
12	7.069	688	694	704	rVV	206995	319379	4.66%	0.750%
13	7.175	707	712	719	rVB5	10304	16758	0.24%	0.039%
14	7.357	737	743	745	rBV3	6660	10456	0.15%	0.025%
15	7.534	766	773	783	rBV	1123975	1747073	25.51%	4.104%
16	8.252	888	895	907	rVB	222578	366157	5.35%	0.860%
17	8.351	907	912	919	rBV	23600	38858	0.57%	0.091%
18	8.687	962	969	977	rBV	186879	309083	4.51%	0.726%
19	9.128	1038	1044	1049	rVB3	5193	8117	0.12%	0.019%
20	9.404	1084	1091	1099	rBV	138250	225552	3.29%	0.530%
21	9.940	1174	1182	1190	rBV	220145	372120	5.43%	0.874%
22	10.104	1203	1210	1218	rBV6	9194	19828	0.29%	0.047%
23	10.310	1238	1245	1260	rVB	1713082	2858332	41.74%	6.714%
24	10.457	1260	1270	1281	rBV	135442	248493	3.63%	0.584%
25	11.910	1512	1517	1522	rVB3	4952	7762	0.11%	0.018%
26	13.028	1701	1707	1714	rVB6	4069	7575	0.11%	0.018%
27	13.610	1800	1806	1817	rBV	513954	692784	10.12%	1.627%
28	13.875	1845	1851	1862	rBV	625389	883485	12.90%	2.075%
29	14.116	1887	1892	1897	rBV5	6260	10065	0.15%	0.024%
30	14.186	1897	1904	1914	rBV	2985980	4284978	62.57%	10.066%
31	14.410	1937	1942	1952	rBV2	49699	98265	1.43%	0.231%
32	14.634	1976	1980	1985	rBV5	15856	23001	0.34%	0.054%
33	15.075	2051	2055	2058	rVB3	8032	8961	0.13%	0.021%
34	15.186	2068	2074	2087	rBV	912721	1265624	18.48%	2.973%
35	15.316	2091	2096	2102	rVV	73850	98120	1.43%	0.230%
36	15.428	2111	2115	2119	rBV5	8437	10852	0.16%	0.025%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102621\
 Data File : BN017121.D
 Acq On : 27 Oct 2021 10:37
 Operator : CG/JU
 Sample : M4215-10
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JDGC9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN102621.M
 Title : SVOA CALIBRATION

37	15.939	2198	2202	2205	rBV3	8298	13731	0.20%	0.032%
38	16.098	2225	2229	2235	rBV4	5865	10824	0.16%	0.025%
39	16.728	2331	2336	2341	rBV2	19842	30736	0.45%	0.072%
40	16.786	2341	2346	2351	rVB4	5802	8567	0.13%	0.020%
41	16.945	2366	2373	2383	rBV	3700169	5379002	78.55%	12.635%
42	17.039	2383	2389	2399	rBV2	1021875	1415257	20.67%	3.324%
43	17.157	2404	2409	2414	rVB4	36830	46690	0.68%	0.110%
44	17.651	2485	2493	2496	rVV2	17379	27326	0.40%	0.064%
45	17.869	2525	2530	2535	rBV3	41784	57076	0.83%	0.134%
46	17.939	2536	2542	2545	rVV3	10211	24209	0.35%	0.057%
47	18.169	2577	2581	2585	rBV5	7458	10298	0.15%	0.024%
48	18.433	2623	2626	2630	rVB3	5441	8126	0.12%	0.019%
49	18.816	2687	2691	2693	rBV3	5835	7559	0.11%	0.018%
50	18.910	2704	2707	2711	rBV3	12830	15266	0.22%	0.036%
51	18.980	2714	2719	2723	rBV3	14126	21228	0.31%	0.050%
52	19.063	2732	2733	2739	rVB3	7067	9252	0.14%	0.022%
53	19.163	2747	2750	2753	rBV3	20566	22898	0.33%	0.054%
54	19.345	2773	2781	2788	rBV	1351298	1854238	27.08%	4.356%
55	19.433	2794	2796	2801	rVB4	13260	16051	0.23%	0.038%
56	19.933	2879	2881	2885	rBV3	15550	16960	0.25%	0.040%
57	20.374	2953	2956	2958	rBV4	14016	15305	0.22%	0.036%
58	20.433	2963	2966	2970	rVV	27543	29878	0.44%	0.070%
59	20.904	3042	3046	3051	rBV	64059	97093	1.42%	0.228%
60	21.098	3076	3079	3083	rBV	38671	42777	0.62%	0.100%
61	21.157	3083	3089	3105	rBV	5150420	6494585	94.84%	15.256%
62	21.339	3117	3120	3124	rBV	69822	74933	1.09%	0.176%
63	21.768	3190	3193	3198	rVB	83906	101338	1.48%	0.238%
64	22.233	3268	3272	3278	rVB	152298	211328	3.09%	0.496%
65	22.733	3353	3357	3368	rVB	218597	355383	5.19%	0.835%
66	23.221	3433	3440	3448	rBV2	1006693	1897714	27.71%	4.458%
67	23.304	3449	3454	3458	rVV	311342	544605	7.95%	1.279%
68	23.362	3458	3464	3481	rVB2	3577377	6847749	100.00%	16.086%
69	23.951	3558	3564	3570	rVB	288620	545138	7.96%	1.281%
70	24.698	3684	3691	3701	rVB	257467	605833	8.85%	1.423%
71	25.568	3833	3839	3851	rVB	174552	462992	6.76%	1.088%
72	26.603	4008	4015	4030	rVB2	131117	396419	5.79%	0.931%




Sum of corrected areas: 42570576

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102621\
Data File : BN017121.D
Acq On : 27 Oct 2021 10:37
Operator : CG/JU
Sample : M4215-10
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JDGC9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN102621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

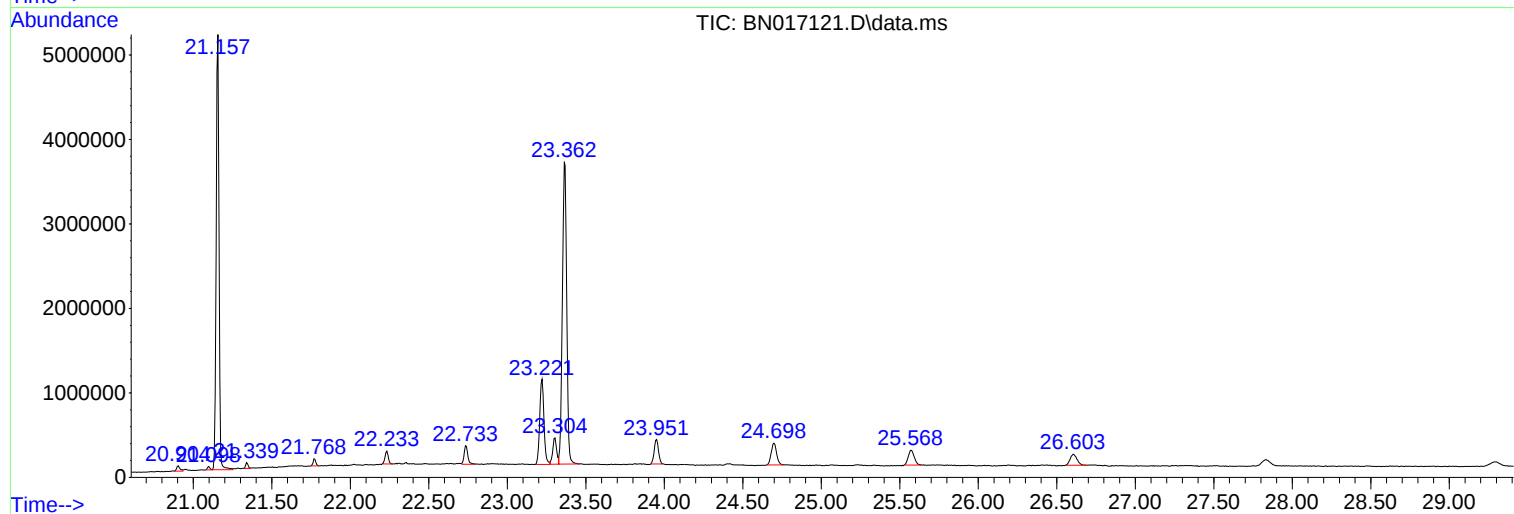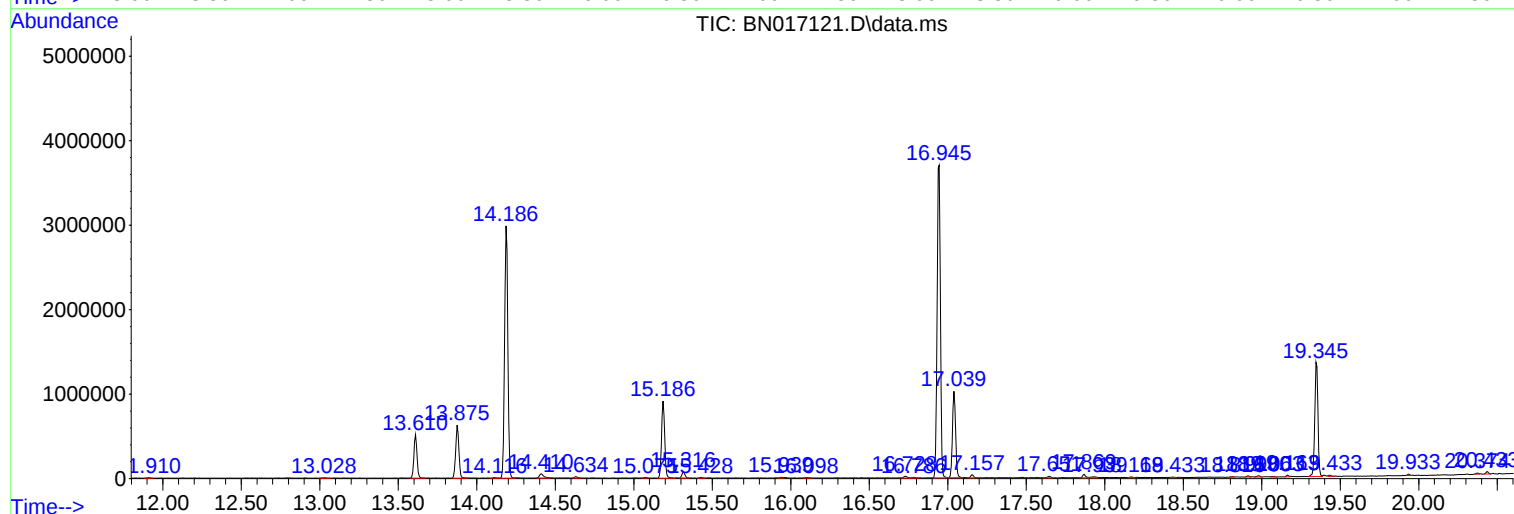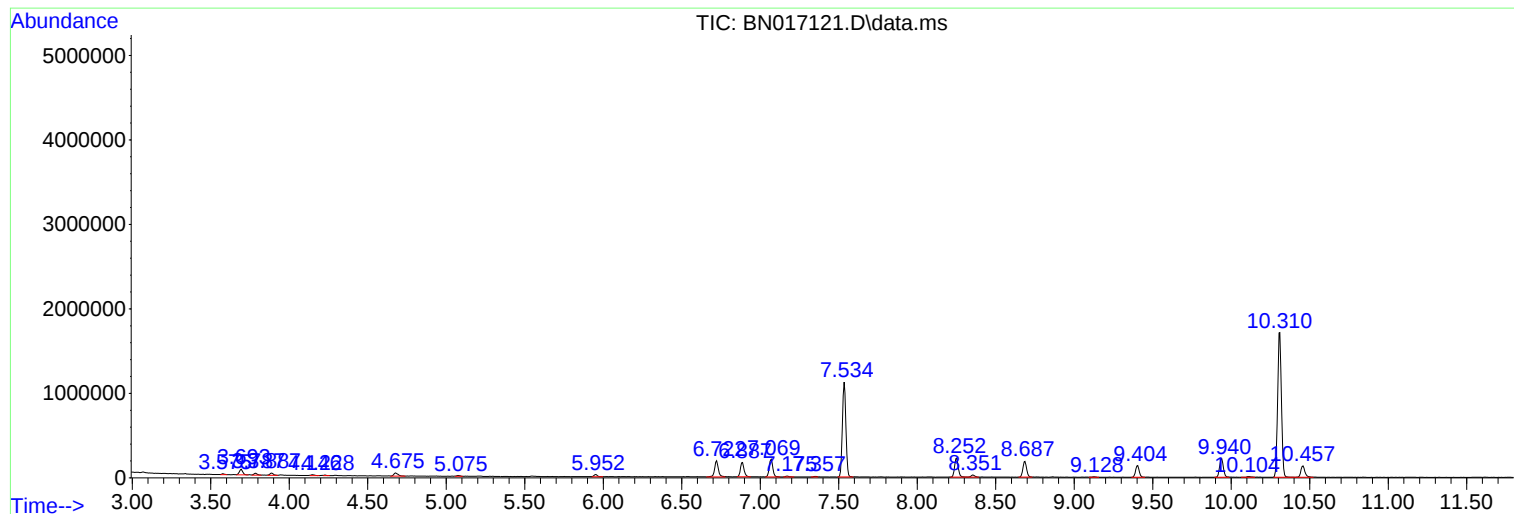

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102621\
Data File : BN017121.D
Acq On : 27 Oct 2021 10:37
Operator : CG/JU
Sample : M4215-10
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JDGC9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN102621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102621\
Data File : BN017121.D
Acq On : 27 Oct 2021 10:37
Operator : CG/JU
Sample : M4215-10
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JDGC9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN102621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
