

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102621\
 Data File : BN017123.D
 Acq On : 27 Oct 2021 11:50
 Operator : CG/JU
 Sample : M4254-05
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Soothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN102621.M
 Title : SVOA CALIBRATION

Signal : TIC: BN017123.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.693	115	120	127	rBV	72951	110336	1.67%	0.347%
2	3.781	132	135	143	rVB	27949	42139	0.64%	0.132%
3	3.887	149	153	160	rVB3	30036	46923	0.71%	0.147%
4	3.946	160	163	169	rVV4	8423	13404	0.20%	0.042%
5	4.005	171	173	180	rVB5	13077	16892	0.26%	0.053%
6	4.146	195	197	202	rVB4	10069	13279	0.20%	0.042%
7	4.410	239	242	248	rVB3	11065	15865	0.24%	0.050%
8	4.675	283	287	296	rVB	36333	59936	0.91%	0.188%
9	5.952	500	504	513	rVB	28670	41991	0.63%	0.132%
10	6.693	625	630	636	rVB4	17214	29234	0.44%	0.092%
11	6.751	636	640	649	rVB	8771	16071	0.24%	0.051%
12	7.175	708	712	716	rBV	8596	10797	0.16%	0.034%
13	7.351	737	742	752	rVB2	6801	13758	0.21%	0.043%
14	7.534	766	773	783	rBV	1141593	1738639	26.26%	5.465%
15	8.357	907	913	921	rBV	41931	73936	1.12%	0.232%
16	9.769	1149	1153	1160	rBV5	6116	10605	0.16%	0.033%
17	10.310	1237	1245	1258	rBV	1712917	2801766	42.32%	8.807%
18	14.186	1898	1904	1916	rBV	2866466	4166823	62.93%	13.098%
19	16.733	2332	2337	2342	rVB	12336	18128	0.27%	0.057%
20	16.945	2366	2373	2385	rBV	3676016	5229119	78.98%	16.437%
21	17.039	2385	2389	2396	rVB2	13667	22981	0.35%	0.072%
22	17.869	2525	2530	2534	rBV6	9263	14768	0.22%	0.046%
23	17.921	2534	2539	2547	rVB4	15763	31639	0.48%	0.099%
24	18.433	2621	2626	2630	rBV	6272	8572	0.13%	0.027%
25	18.663	2662	2665	2670	rVB	9012	11619	0.18%	0.037%
26	18.968	2715	2717	2723	rVB4	8022	10261	0.15%	0.032%
27	19.168	2746	2751	2752	rBV4	5675	6994	0.11%	0.022%
28	19.316	2768	2776	2779	rBV6	24272	45449	0.69%	0.143%
29	19.351	2779	2782	2783	rBV3	6521	7178	0.11%	0.023%
30	19.433	2786	2796	2801	rBV3	41352	140221	2.12%	0.441%
31	19.533	2811	2813	2814	rBV2	12444	9401	0.14%	0.030%
32	19.580	2814	2821	2822	rBV3	59129	106876	1.61%	0.336%
33	19.604	2822	2825	2826	rBV2	33150	34720	0.52%	0.109%
34	19.674	2835	2837	2860	rVB3	233791	697689	10.54%	2.193%
35	19.992	2889	2891	2893	rBV3	5600	7156	0.11%	0.022%
36	20.057	2893	2902	2908	rVV3	15720	57003	0.86%	0.179%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102621\
 Data File : BN017123.D
 Acq On : 27 Oct 2021 11:50
 Operator : CG/JU
 Sample : M4254-05
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN102621.M
 Title : SVOA CALIBRATION

37	20.368	2951	2955	2962	rBV3	34158	60061	0.91%	0.189%
38	20.433	2964	2966	2971	rVV4	9407	12558	0.19%	0.039%
39	20.739	3015	3018	3022	rVB5	7382	7986	0.12%	0.025%
40	20.904	3043	3046	3050	rBV4	15857	20097	0.30%	0.063%
41	20.951	3052	3054	3059	rVB6	9885	11562	0.17%	0.036%
42	21.098	3076	3079	3083	rBV2	16198	16446	0.25%	0.052%
43	21.157	3083	3089	3104	rBV	4926916	6229734	94.09%	19.582%
44	21.339	3117	3120	3123	rBV	27180	28088	0.42%	0.088%
45	21.774	3190	3194	3197	rBV	49846	55750	0.84%	0.175%
46	22.233	3268	3272	3276	rVB	107168	135590	2.05%	0.426%
47	22.739	3353	3358	3364	rVB	200510	292039	4.41%	0.918%
48	23.304	3448	3454	3458	rBV	306534	522062	7.88%	1.641%
49	23.362	3458	3464	3481	rVB2	3461884	6621151	100.00%	20.813%
50	23.951	3558	3564	3573	rVB	316453	600493	9.07%	1.888%
51	24.698	3684	3691	3699	rBV2	275639	621385	9.38%	1.953%
52	25.574	3833	3840	3850	rVB2	181018	463070	6.99%	1.456%
53	26.603	4008	4015	4031	rVB3	137650	432866	6.54%	1.361%




Sum of corrected areas: 31813106

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102621\
Data File : BN017123.D
Acq On : 27 Oct 2021 11:50
Operator : CG/JU
Sample : M4254-05
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN102621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

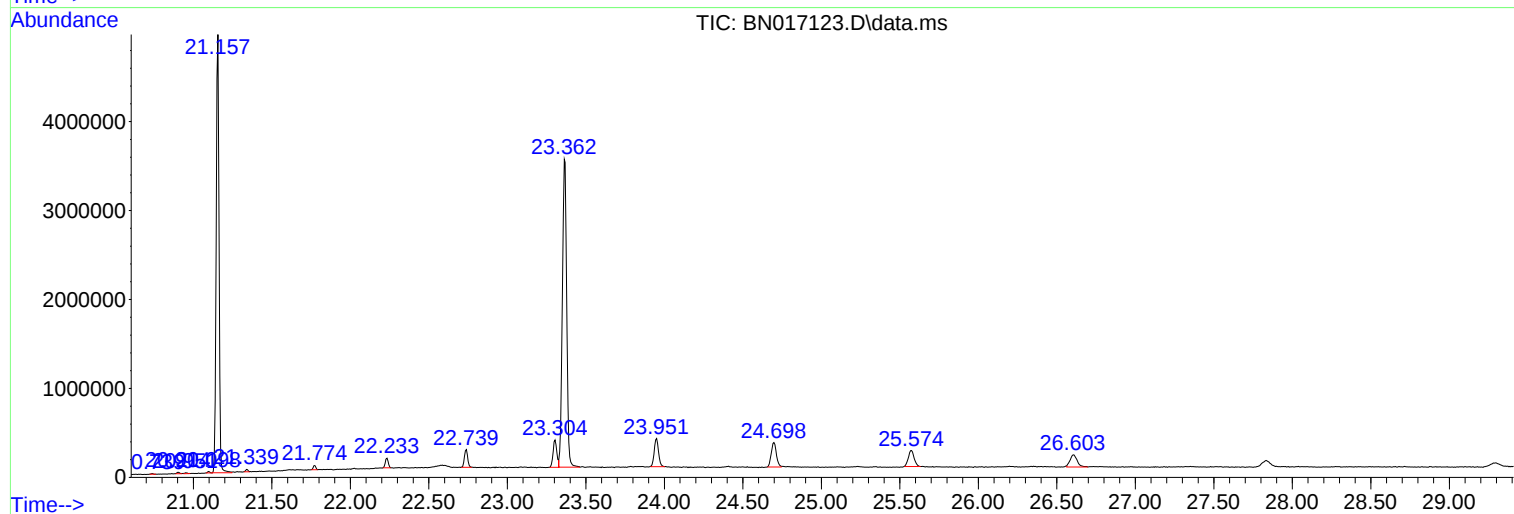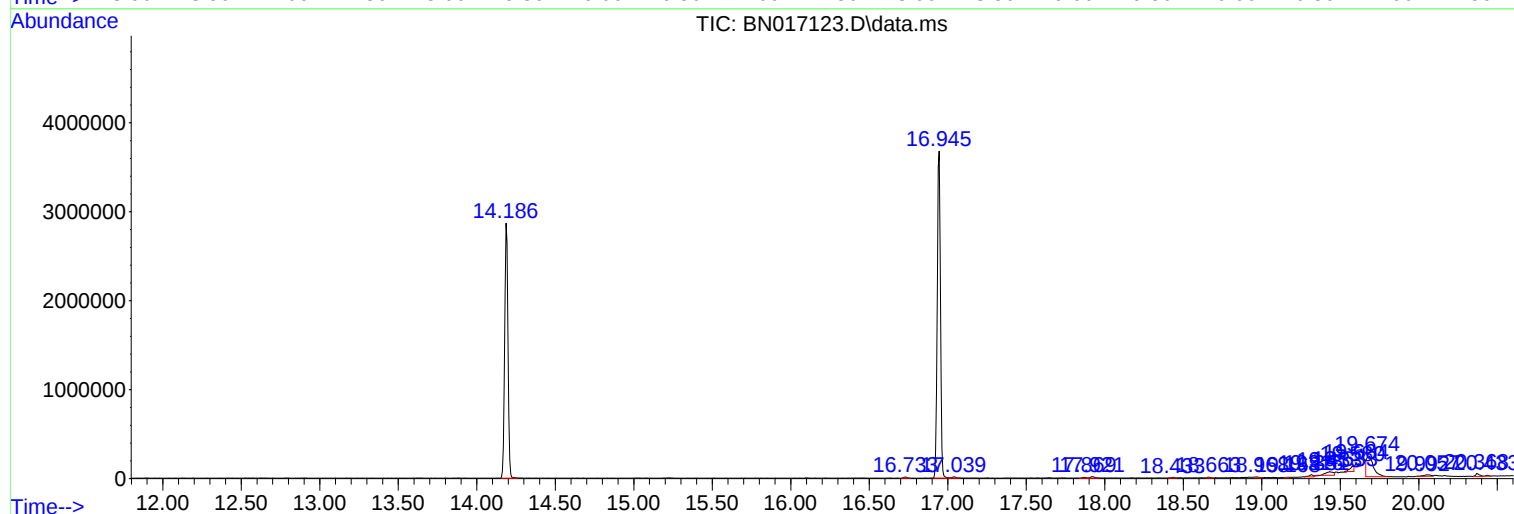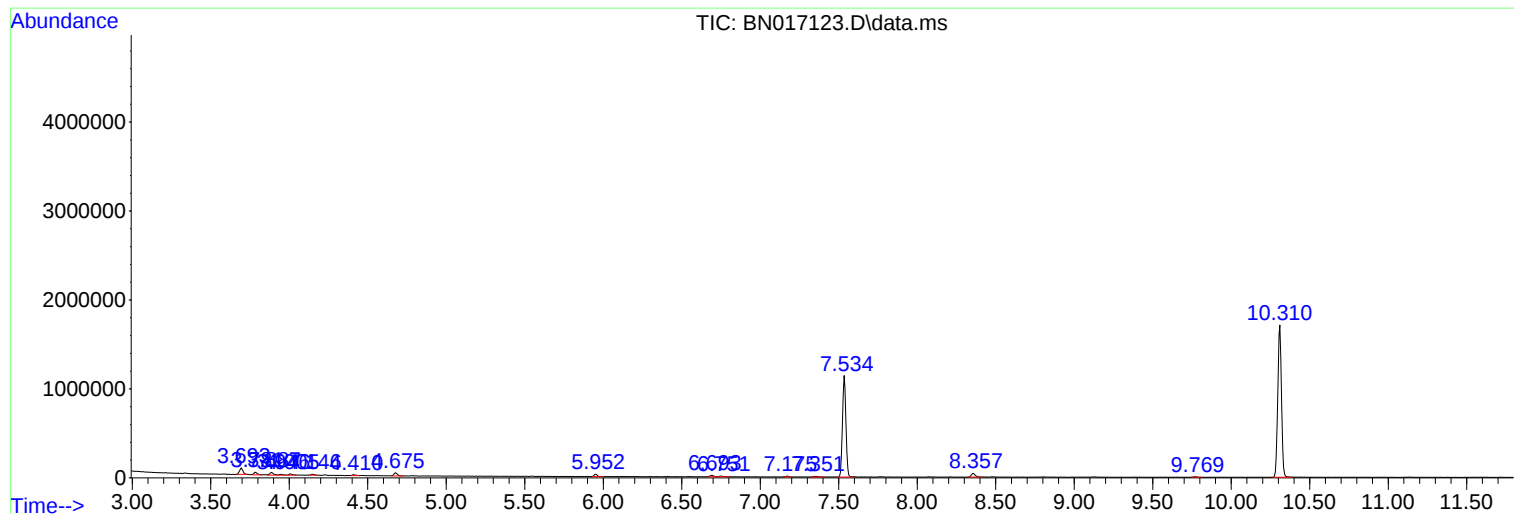

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102621\
Data File : BN017123.D
Acq On : 27 Oct 2021 11:50
Operator : CG/JU
Sample : M4254-05
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN102621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(3S,6aR,6bR,8aS...	19.674	2.2	ng/u1	697689	5	21.157	6229730	20.0