

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102621\
 Data File : BN017128.D
 Acq On : 27 Oct 2021 14:54
 Operator : CG/JU
 Sample : M4215-07
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JDGC6

Integration Parameters: LSCINT.P

Integrator: RTE

Smothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN102621.M
 Title : SVOA CALIBRATION

Signal : TIC: BN017128.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.070	11	14	20	rVB	18906	25452	0.39%	0.051%
2	3.470	78	82	92	rBV	97745	179619	2.74%	0.363%
3	3.575	97	100	108	rVB5	14174	25479	0.39%	0.051%
4	3.693	115	120	127	rVB	65339	99651	1.52%	0.201%
5	3.781	132	135	142	rVB	16979	24985	0.38%	0.050%
6	3.887	149	153	160	rVB3	27491	41985	0.64%	0.085%
7	4.146	194	197	207	rVV6	11165	15570	0.24%	0.031%
8	4.675	281	287	293	rBV	35811	53622	0.82%	0.108%
9	5.646	449	452	457	rBV3	4201	6580	0.10%	0.013%
10	5.952	499	504	509	rBV2	25088	35474	0.54%	0.072%
11	6.722	625	635	643	rBV	329008	536872	8.20%	1.084%
12	6.887	655	663	672	rBV	281615	449700	6.87%	0.908%
13	7.069	687	694	702	rBV	363452	550488	8.41%	1.112%
14	7.169	707	711	718	rBV4	9743	16454	0.25%	0.033%
15	7.352	737	742	747	rBV	6336	10706	0.16%	0.022%
16	7.534	767	773	782	rBV	1139253	1770564	27.05%	3.576%
17	7.605	784	785	792	rVV4	6082	8391	0.13%	0.017%
18	7.763	808	812	816	rBV3	7718	11987	0.18%	0.024%
19	8.075	861	865	869	rBV3	6409	10794	0.16%	0.022%
20	8.252	889	895	905	rVB	342550	546761	8.35%	1.104%
21	8.352	908	912	920	rVB	24054	38844	0.59%	0.078%
22	8.687	962	969	978	rBV	321667	523024	7.99%	1.056%
23	9.122	1038	1043	1050	rBV5	7407	12780	0.20%	0.026%
24	9.405	1084	1091	1103	rVB	258185	427172	6.53%	0.863%
25	9.934	1175	1181	1192	rBV	406885	662427	10.12%	1.338%
26	10.105	1205	1210	1222	rBV	72418	131633	2.01%	0.266%
27	10.310	1237	1245	1256	rVB	1751831	2907835	44.42%	5.873%
28	10.452	1263	1269	1283	rBV	395385	695915	10.63%	1.406%
29	11.910	1513	1517	1524	rVB	7709	12990	0.20%	0.026%
30	12.534	1616	1623	1627	rBV5	3890	6831	0.10%	0.014%
31	12.798	1662	1668	1671	rBV4	5965	7899	0.12%	0.016%
32	13.104	1713	1720	1724	rVV6	3793	6588	0.10%	0.013%
33	13.610	1800	1806	1816	rBV	912024	1229581	18.78%	2.483%
34	13.875	1845	1851	1861	rBV	1034844	1456774	22.25%	2.942%
35	14.187	1897	1904	1912	rBV	2944176	4316993	65.95%	8.719%
36	14.410	1936	1942	1959	rBV	230275	398182	6.08%	0.804%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102621\
 Data File : BN017128.D
 Acq On : 27 Oct 2021 14:54
 Operator : CG/JU
 Sample : M4215-07
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JDGC6

Integration Parameters: LSCINT.P

Integrator: RTE

Soothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN102621.M
 Title : SVOA CALIBRATION

37	14.628	1975	1979	1987	rVB3	33122	49058	0.75%	0.099%
38	15.187	2068	2074	2086	rBV	1412623	1982200	30.28%	4.004%
39	15.316	2090	2096	2105	rBV	268228	354100	5.41%	0.715%
40	15.428	2111	2115	2119	rVB2	12397	16305	0.25%	0.033%
41	16.104	2223	2230	2236	rBV9	4985	8317	0.13%	0.017%
42	16.504	2294	2298	2302	rBV	12004	13410	0.20%	0.027%
43	16.728	2331	2336	2343	rBV	16742	26206	0.40%	0.053%
44	16.945	2366	2373	2381	rBV	3714058	5344534	81.64%	10.795%
45	17.039	2383	2389	2399	rBV	1571689	2147034	32.80%	4.337%
46	17.157	2404	2409	2415	rVB2	69638	88162	1.35%	0.178%
47	17.651	2488	2493	2497	rBV2	15078	18789	0.29%	0.038%
48	17.869	2525	2530	2533	rBV2	38618	47234	0.72%	0.095%
49	17.939	2537	2542	2546	rVB3	9299	16365	0.25%	0.033%
50	18.428	2622	2625	2632	rBV7	4485	9314	0.14%	0.019%
51	18.828	2691	2693	2698	rVB6	7854	10064	0.15%	0.020%
52	18.910	2703	2707	2712	rVV2	21422	31432	0.48%	0.063%
53	18.981	2715	2719	2723	rVB	20517	29333	0.45%	0.059%
54	19.163	2747	2750	2754	rBV5	8230	11383	0.17%	0.023%
55	19.345	2772	2781	2788	rBV	2137920	2877616	43.96%	5.812%
56	19.933	2878	2881	2884	rVV2	15789	17319	0.26%	0.035%
57	20.369	2953	2955	2961	rVB4	16603	19285	0.29%	0.039%
58	20.433	2963	2966	2970	rVB	27503	30232	0.46%	0.061%
59	20.733	3014	3017	3020	rBV5	11329	15529	0.24%	0.031%
60	20.898	3041	3045	3052	rBV	100385	171962	2.63%	0.347%
61	21.098	3076	3079	3082	rBV	23906	25941	0.40%	0.052%
62	21.157	3083	3089	3100	rVV	4648155	6192837	94.60%	12.508%
63	21.339	3117	3120	3124	rVB	79035	79170	1.21%	0.160%
64	21.769	3190	3193	3198	rVB	100615	113290	1.73%	0.229%
65	22.227	3265	3271	3277	rBV2	232229	406415	6.21%	0.821%
66	22.733	3353	3357	3363	rVB	223953	312035	4.77%	0.630%
67	23.221	3433	3440	3448	rBV2	1591918	2871273	43.86%	5.799%
68	23.298	3449	3453	3457	rVV	288358	482491	7.37%	0.975%
69	23.363	3457	3464	3480	rVB2	3477907	6546234	100.00%	13.222%
70	23.945	3557	3563	3575	rVB2	282296	566245	8.65%	1.144%
71	24.692	3684	3690	3703	rVB	237399	555923	8.49%	1.123%
72	25.568	3833	3839	3851	rVB	165382	431129	6.59%	0.871%
73	26.604	4009	4015	4026	rVB2	115887	335586	5.13%	0.678%




Sum of corrected areas: 49510354

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102621\
Data File : BN017128.D
Acq On : 27 Oct 2021 14:54
Operator : CG/JU
Sample : M4215-07
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JDGC6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN102621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

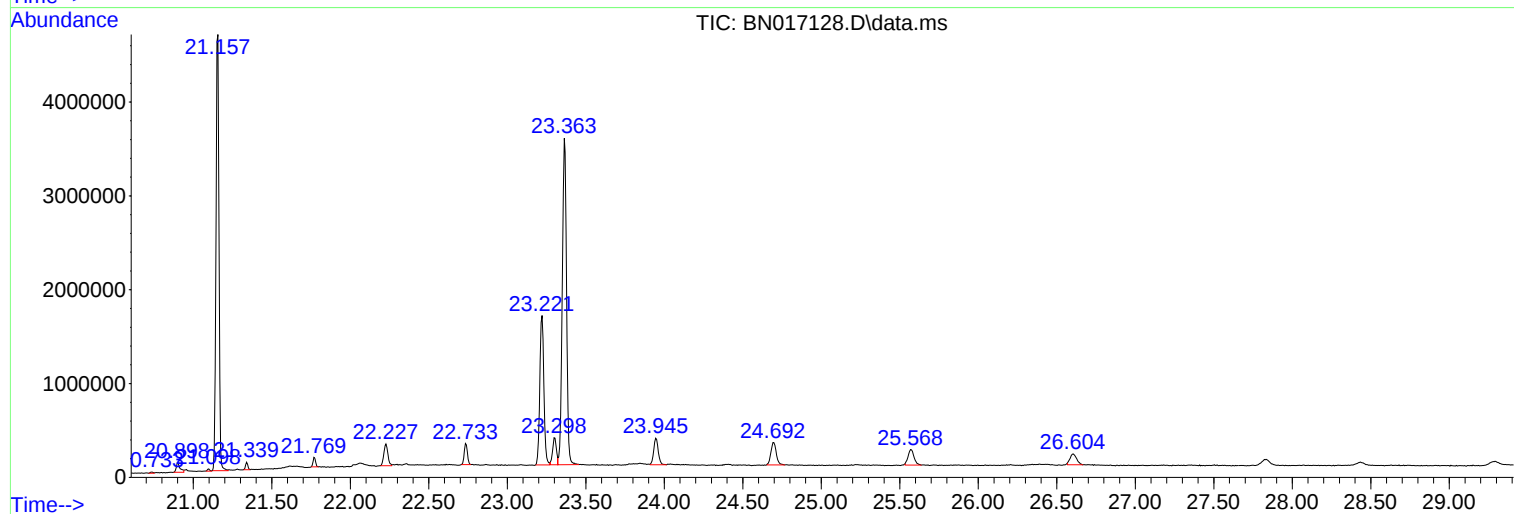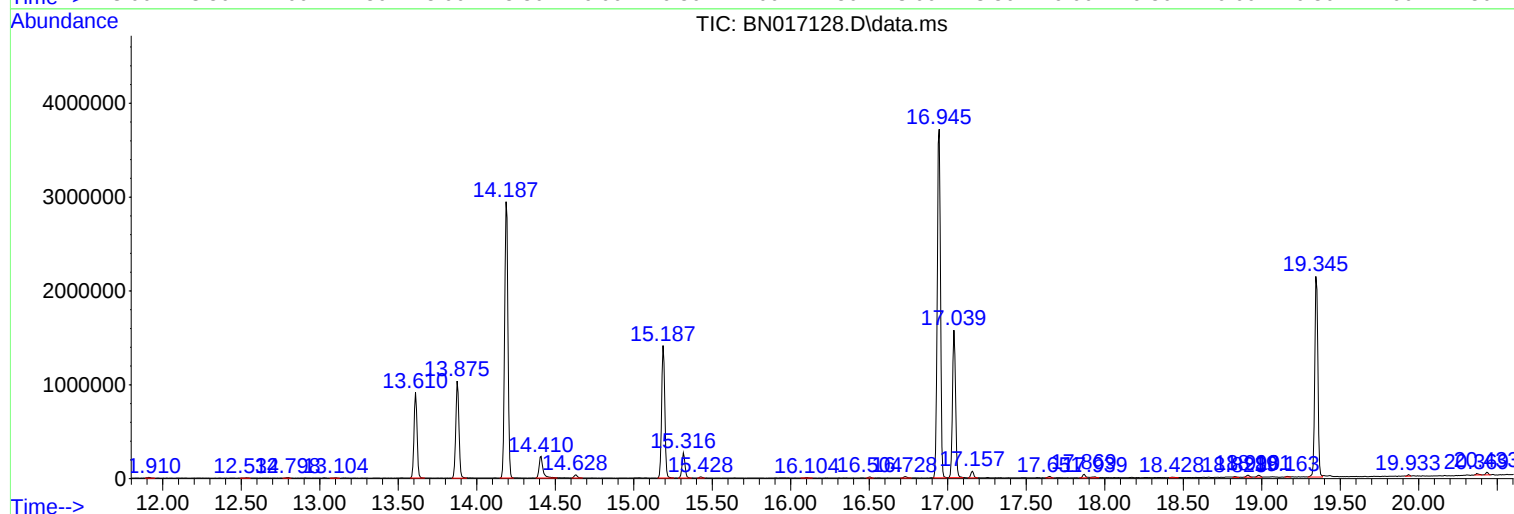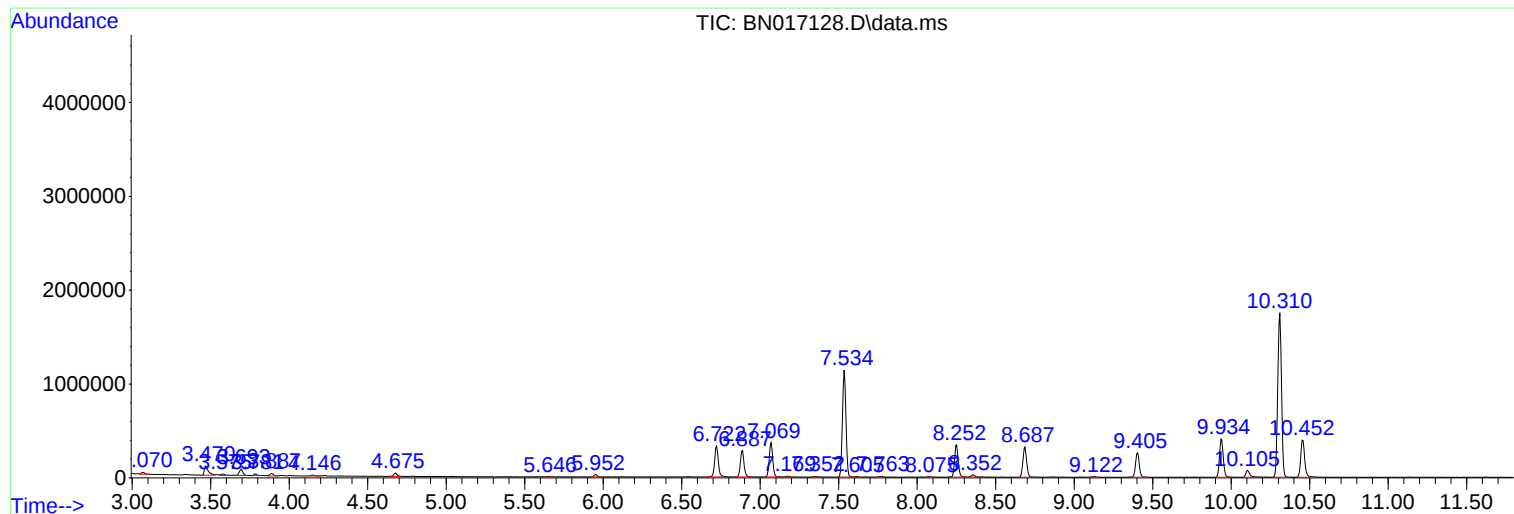

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102621\
Data File : BN017128.D
Acq On : 27 Oct 2021 14:54
Operator : CG/JU
Sample : M4215-07
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JDGC6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN102621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102621\
Data File : BN017128.D
Acq On : 27 Oct 2021 14:54
Operator : CG/JU
Sample : M4215-07
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JDGC6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN102621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------