
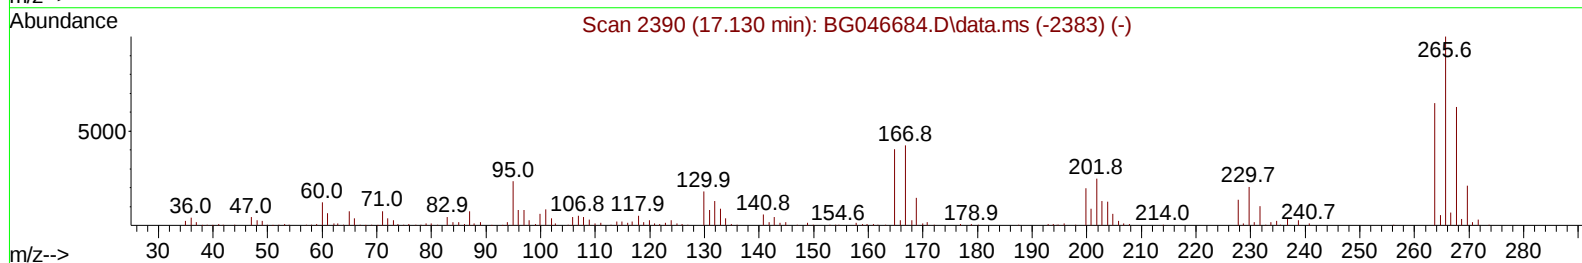
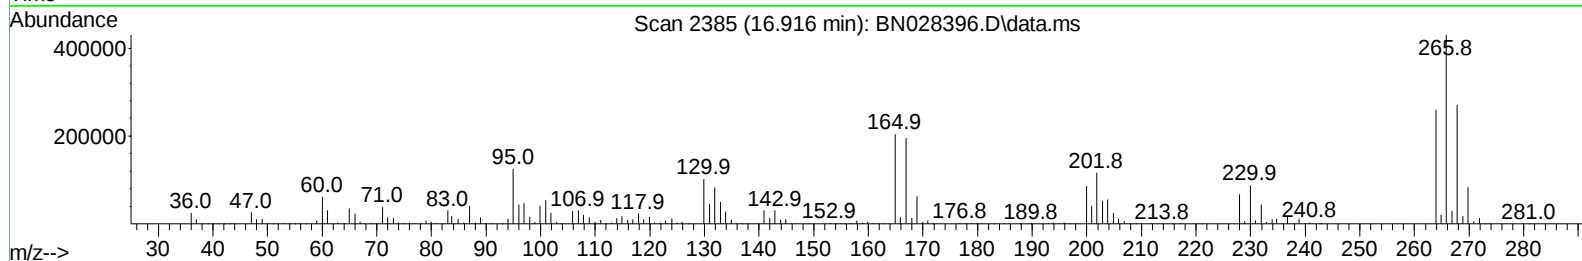


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102623\
Data File : BN028396.D
Acq On : 26 Oct 2023 13:33
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 27 05:01:20 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 27 05:01:16 2023
Response via : Initial Calibration

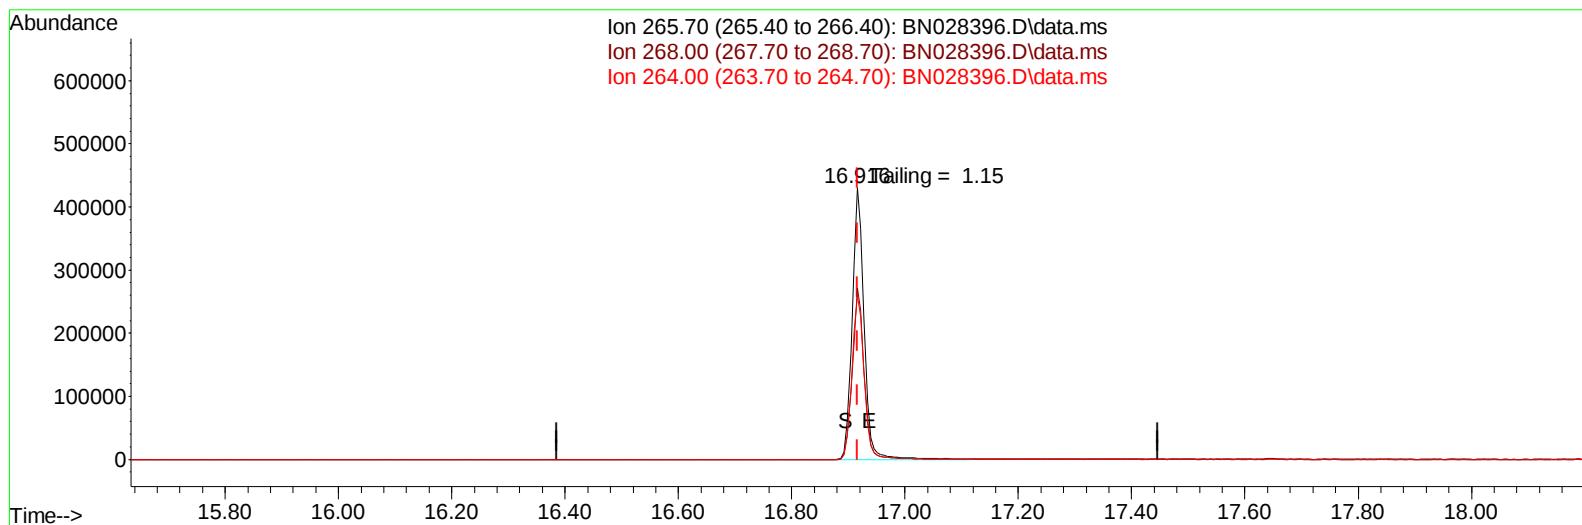




TIC: BN028396.D\data.ms

(70) Pentachlorophenol (C)**16.916min (0.000) 19666.98 ng****response 634961**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.09
264.00	61.60	60.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102623\
Data File : BN028396.D
Acq On : 26 Oct 2023 13:33
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 27 05:01:20 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 27 05:01:16 2023
Response via : Initial Calibration

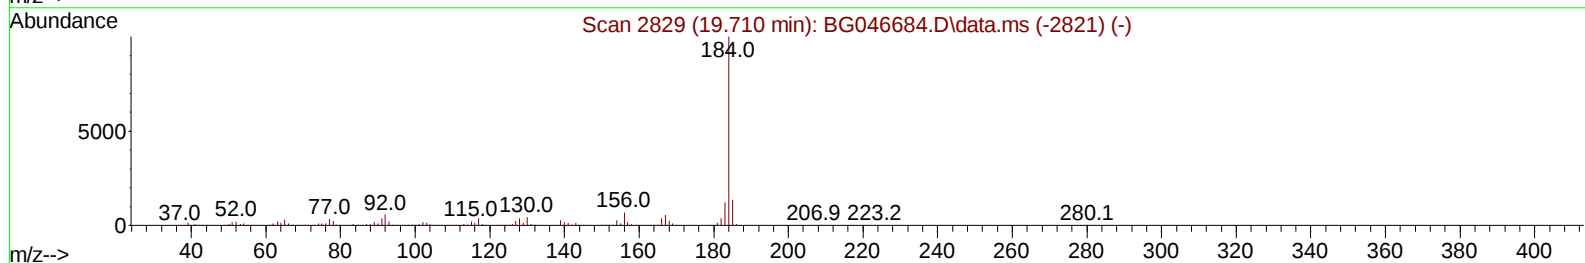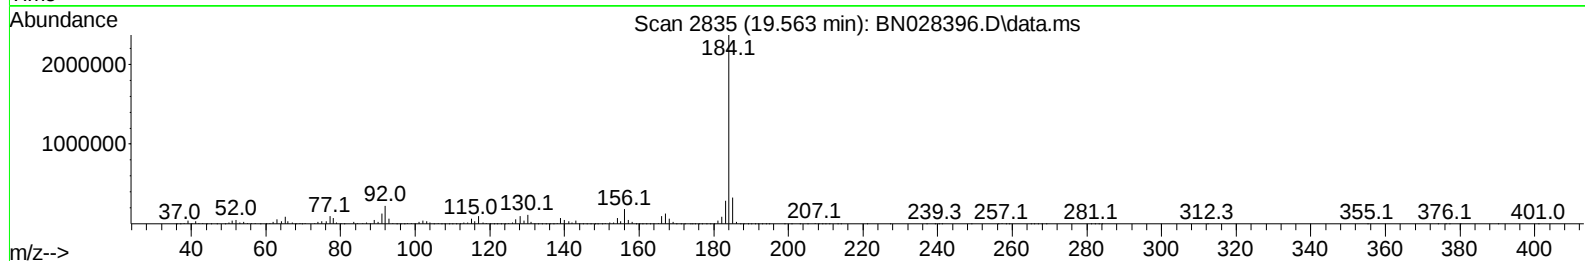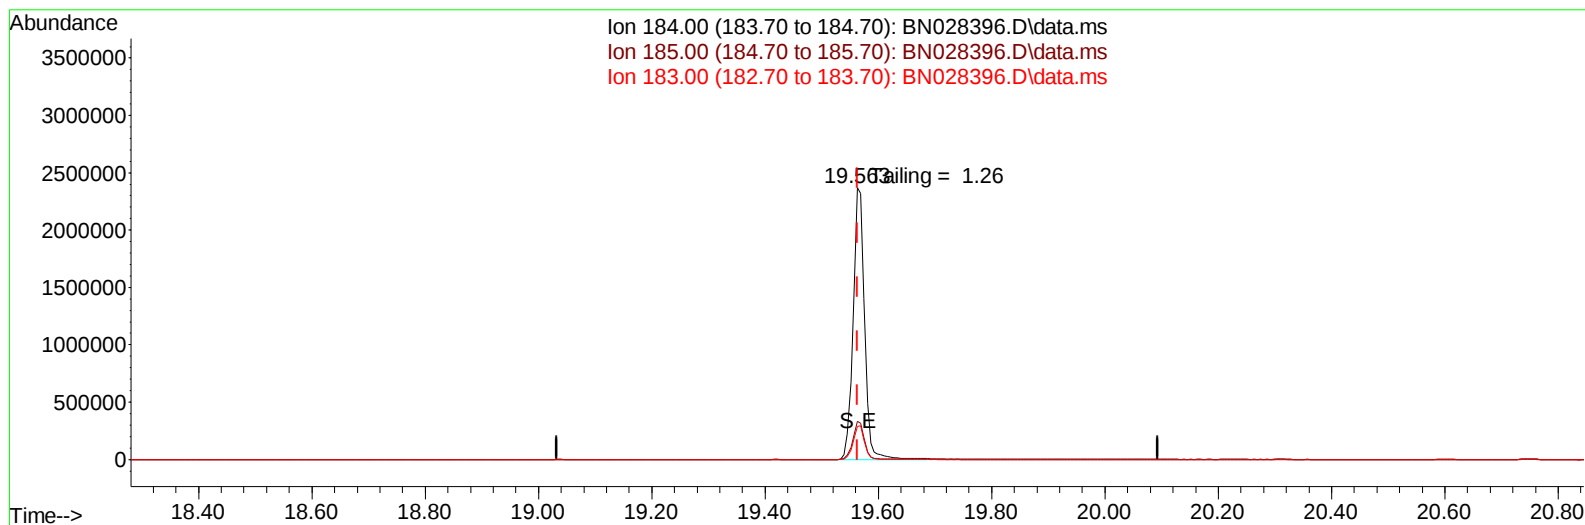

TIC: BN028396.D\data.ms

(77) Benzidine

19.563min (0.000) 610285.92 ng

response 3367400

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.94
183.00	13.20	12.12
0.00	0.00	0.00