
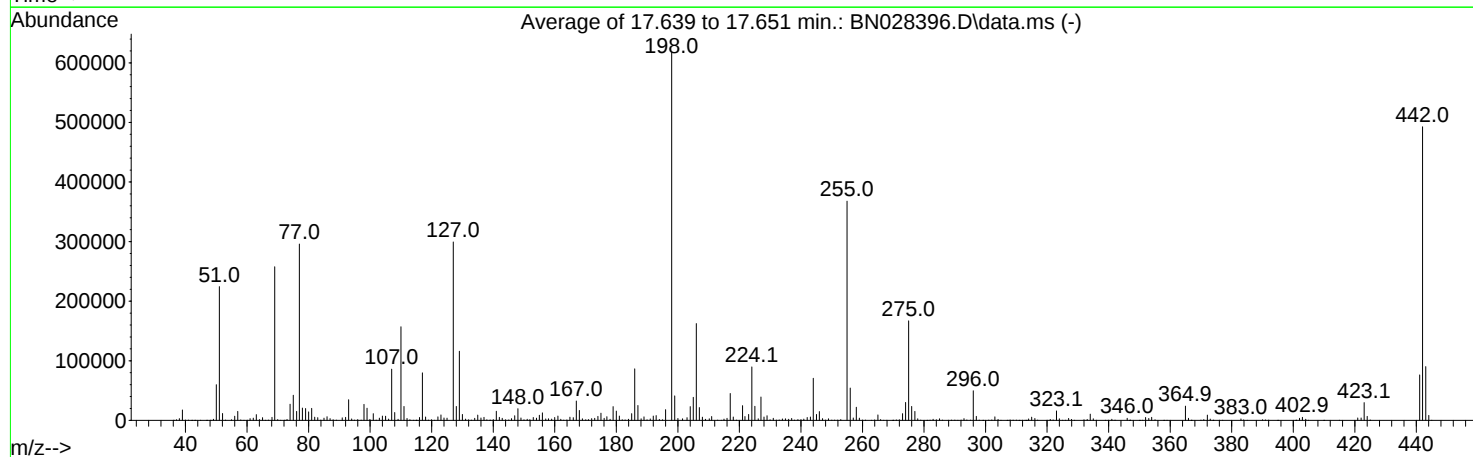


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102623\
Data File : BN028396.D
Acq On : 26 Oct 2023 13:33
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN101223.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Oct 23 15:14:08 2023

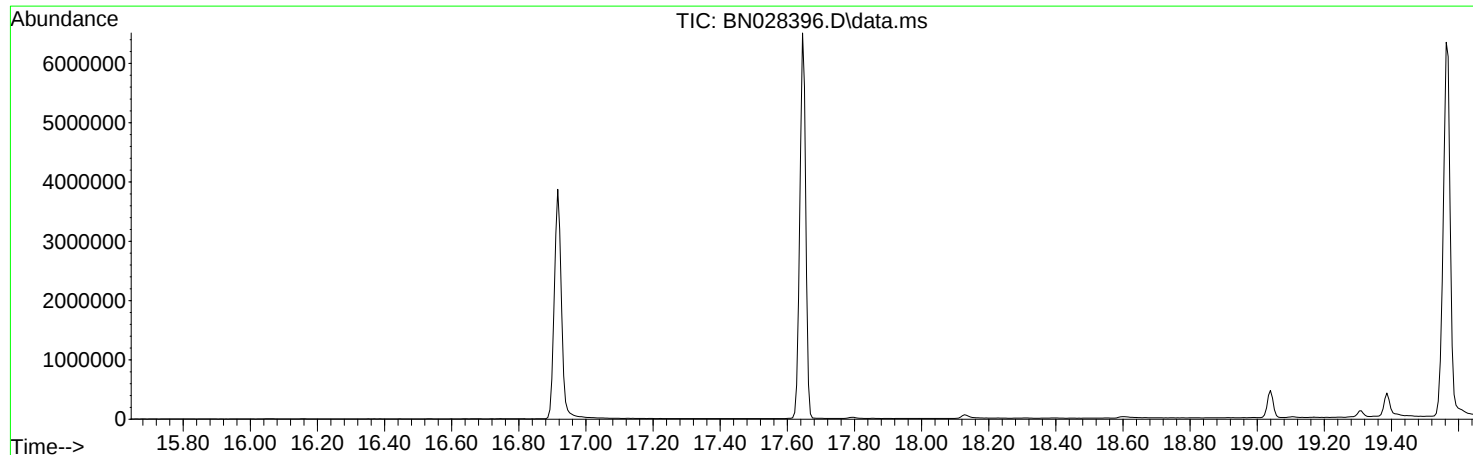




AutoFind: Scans 2508, 2509, 2510; Background Corrected with Scan 2501

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.4	224513	PASS
68	69	0.00	2	2.0	5034	PASS
69	198	0.00	100	41.8	257891	PASS
70	69	0.00	2	0.6	1449	PASS
127	198	10	80	48.5	299413	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	617344	PASS
199	198	5	9	6.7	41163	PASS
275	198	10	60	27.0	166933	PASS
365	198	1	100	3.9	23848	PASS
441	198	0.01	100	12.3	76200	PASS
442	442	50	100	100.0	492608	PASS
443	442	15	24	18.3	90355	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102623\
 Data File : BN028396.D
 Acq On : 26 Oct 2023 13:33
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Oct 27 05:01:20 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 27 05:01:16 2023
 Response via : Initial Calibration

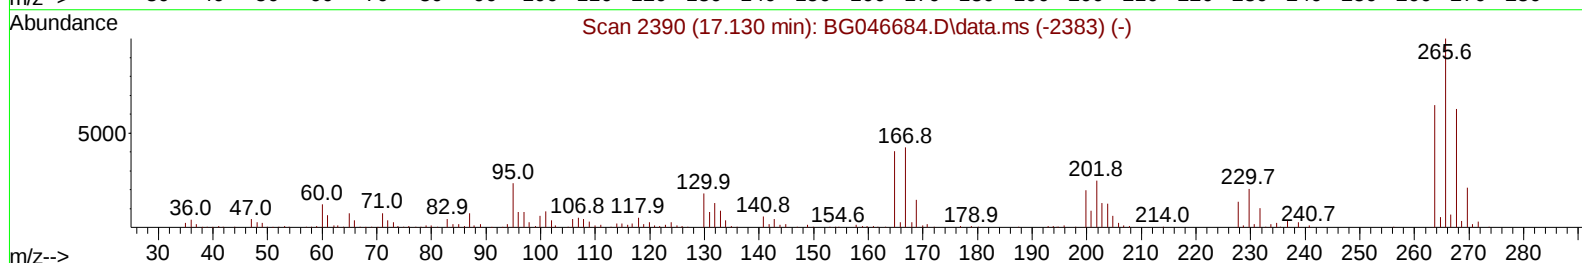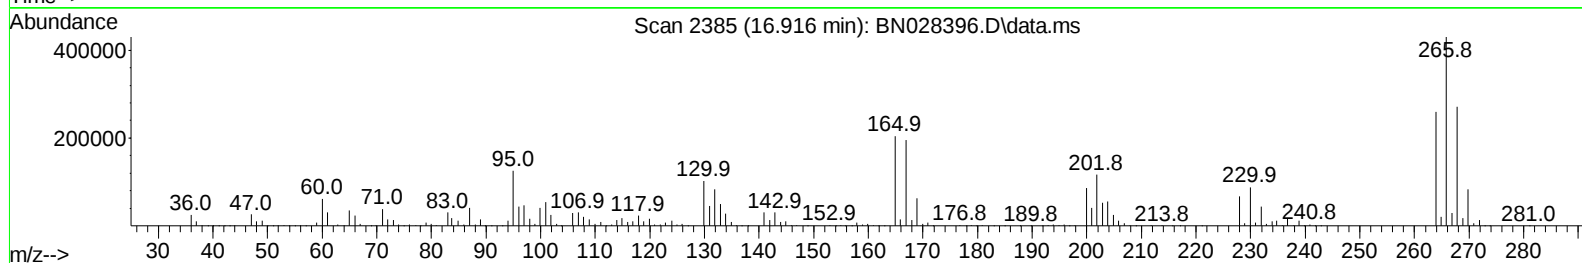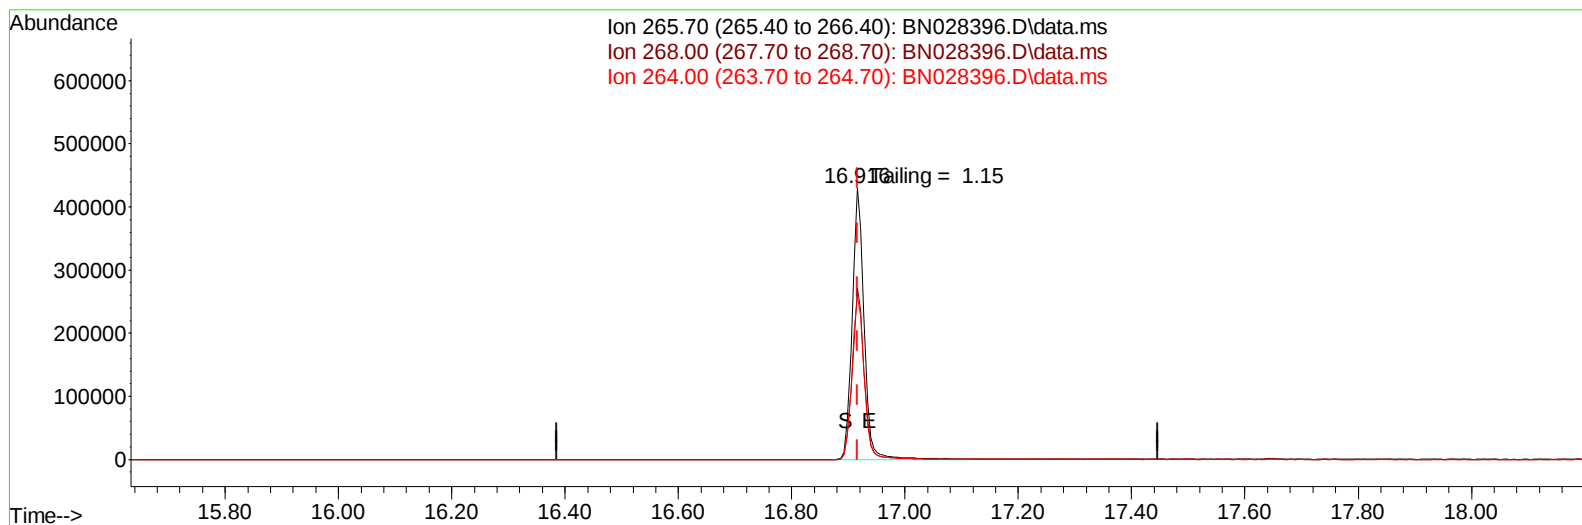

TIC: BN028396.D\data.ms

(70) Pentachlorophenol (C)

16.916min (0.000) 19666.98 ng




response 634961

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.09
264.00	61.60	60.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102623\
Data File : BN028396.D
Acq On : 26 Oct 2023 13:33
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 27 05:01:20 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 27 05:01:16 2023
Response via : Initial Calibration

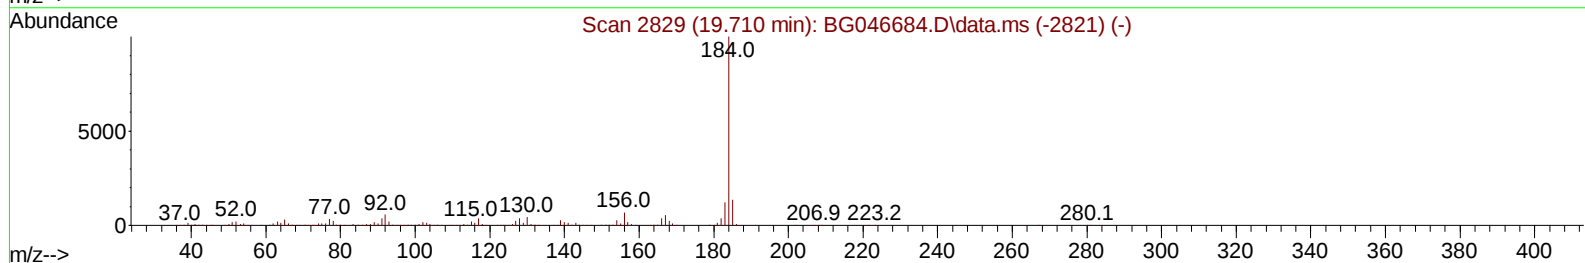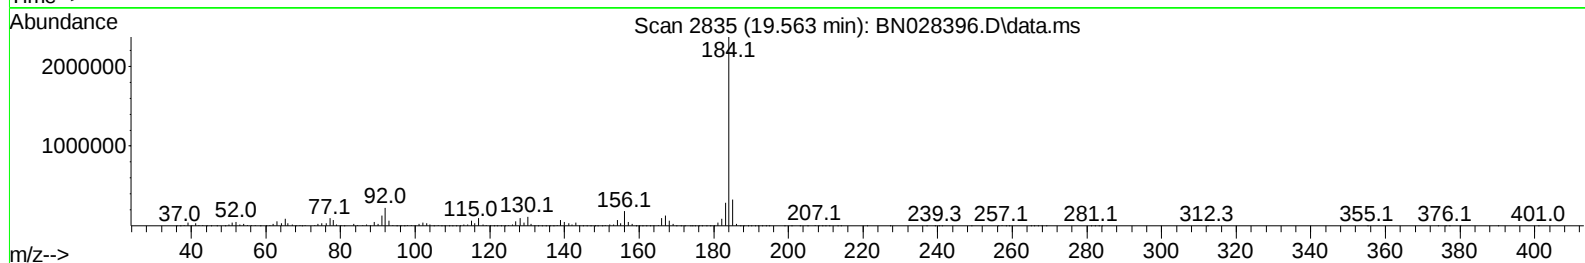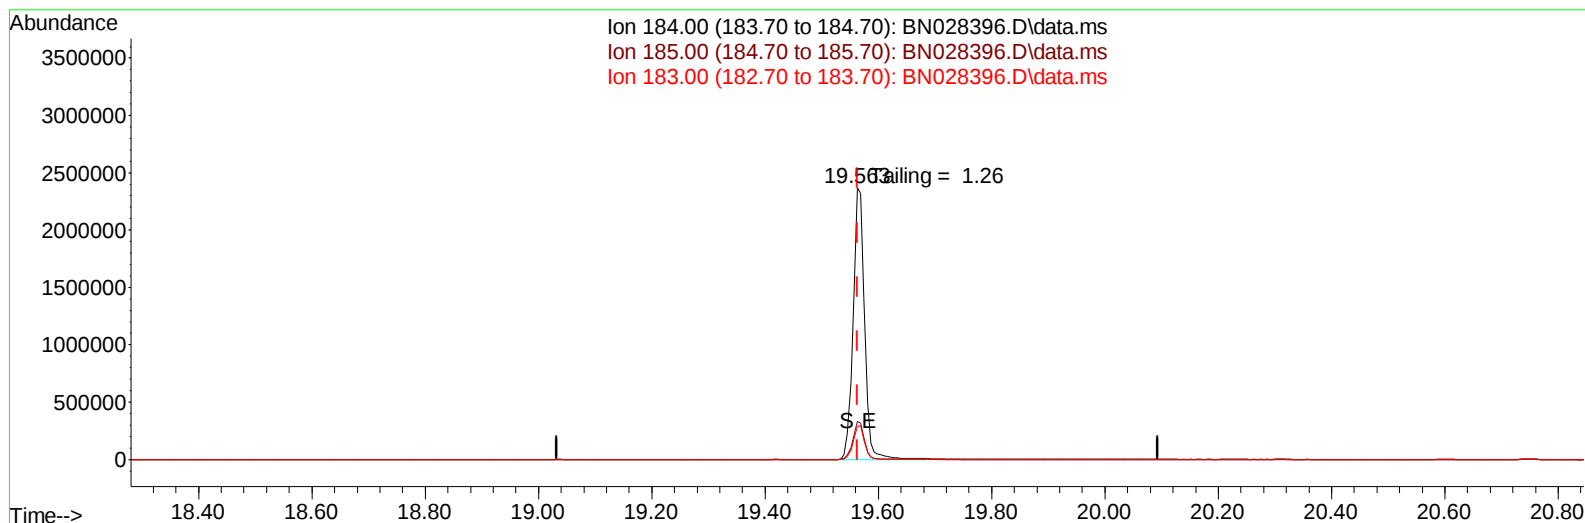

TIC: BN028396.D\data.ms

(77) Benzidine

19.563min (0.000) 610285.92 ng

response 3367400

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.94
183.00	13.20	12.12
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/26/2023	BNA_N	<u>BN028396.D</u>
Compound Name	Response	Retention Time
DDT	1036643	20.751
DDD	399302	20.316
DDE	4445	19.792
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
403747	1440390	28.03

Instrument :
BNA_N
ClientSampleId :
DFTPP