


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN102819\
Data File : BN008438.D
Acq On : 28 Oct 2019 13:22
Operator : JU
Sample : PB123997BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK97

Manual Integrations
APPROVED

mohammad
10/29/2019 3:36:17 PM

Quant Time: Oct 29 11:29:19 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 25 13:14:06 2019
Response via : Initial Calibration

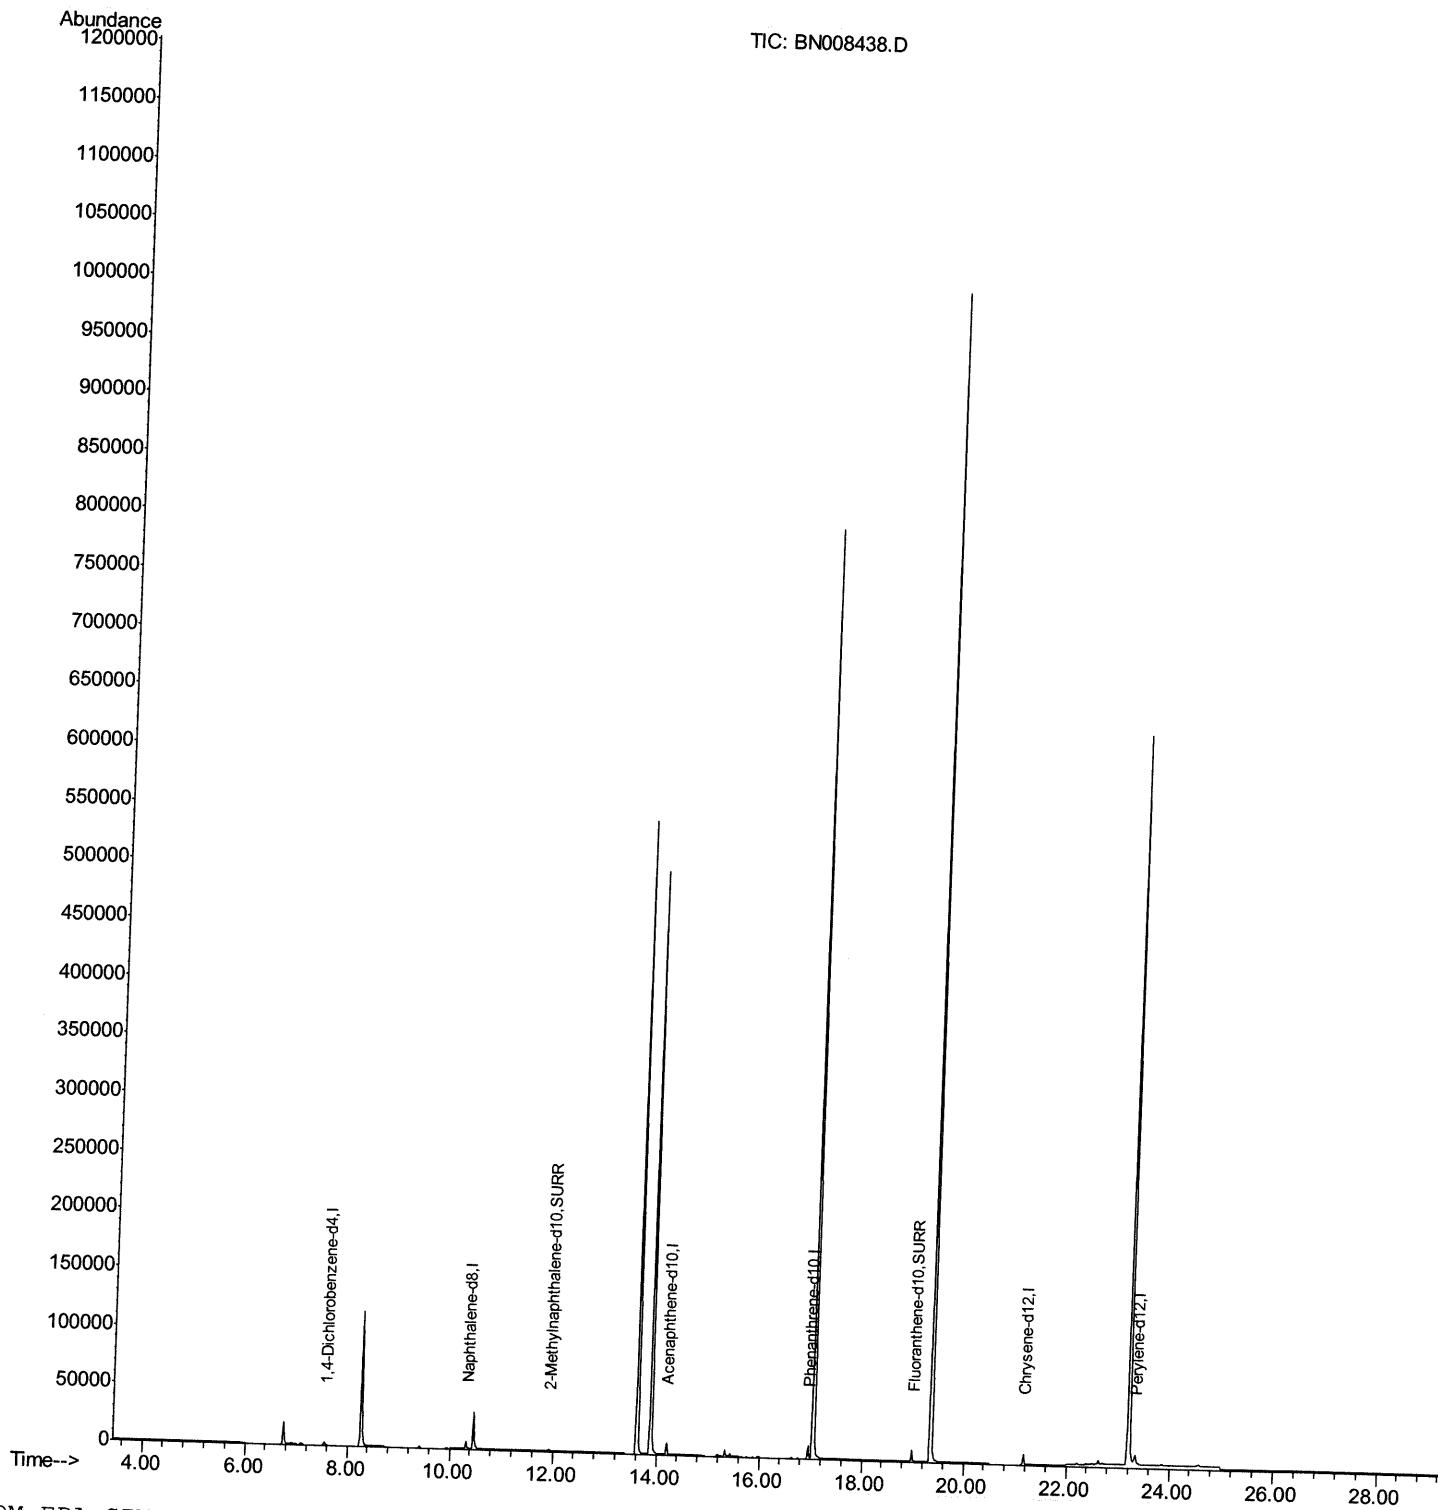


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN102819\
Data File : BN008438.D
Acq On : 28 Oct 2019 13:22
Operator : JU
Sample : PB123997BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK97

Manual Integrations
APPROVED

mohammad
10/29/2019 3:36:17 PM

Quant Time: Oct 29 11:28:04 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 25 13:14:06 2019
Response via : Initial Calibration

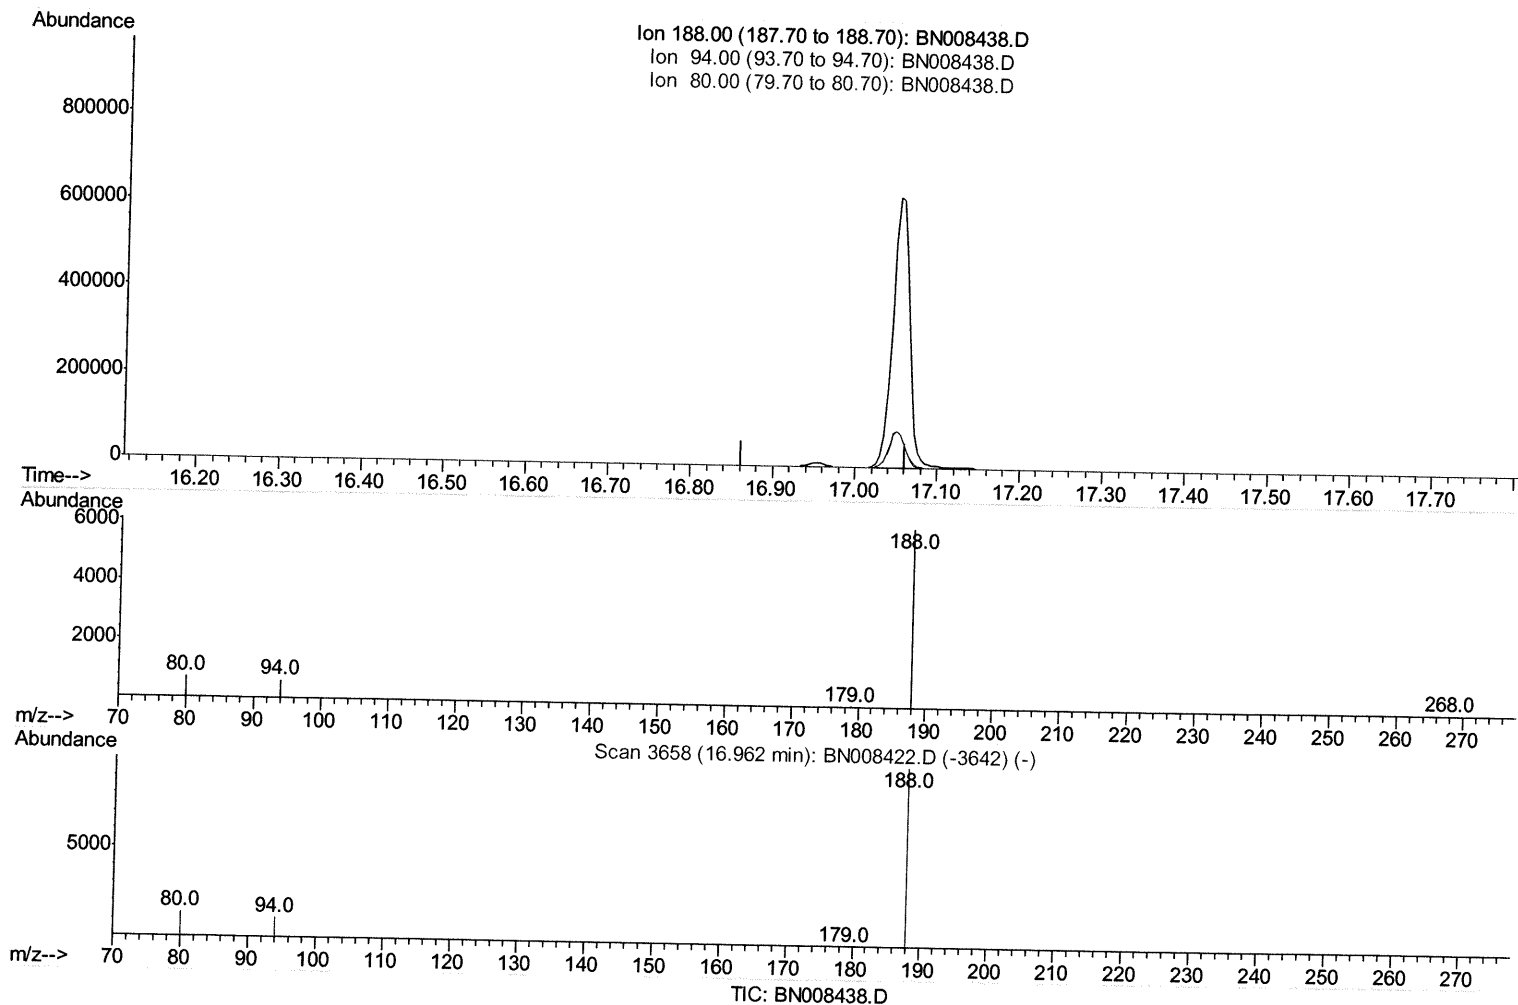

(10) Phenanthrene-d10 (I)

16.962min (-16.962) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	10.90	0.00#
80.00	12.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN102819\
 Data File : BN008438.D
 Acq On : 28 Oct 2019 13:22
 Operator : JU
 Sample : PB123997BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK97

Manual Integrations
 APPROVED

mohammad
 10/29/2019 3:36:17 PM

Quant Time: Oct 29 11:28:04 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 25 13:14:06 2019
 Response via : Initial Calibration

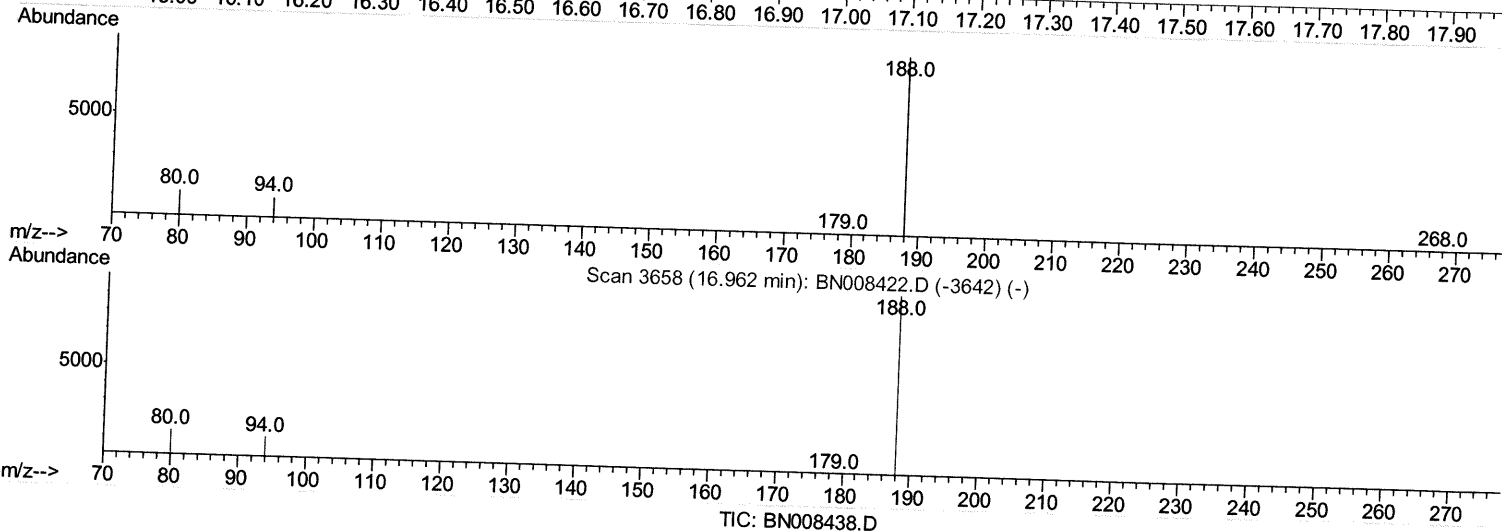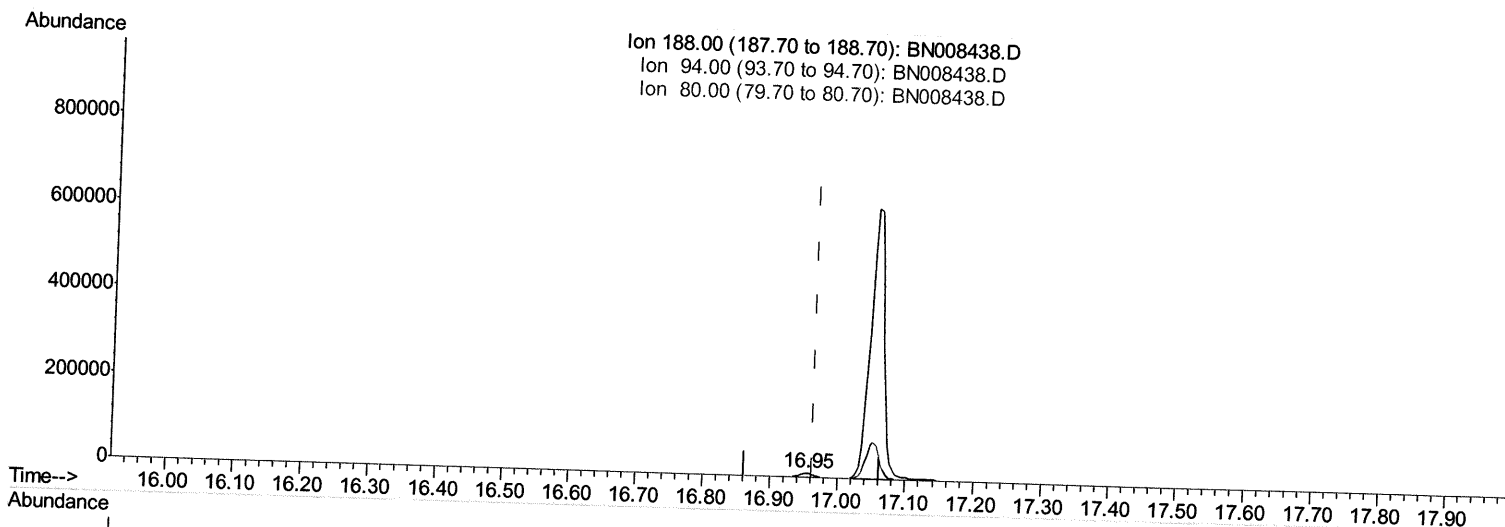

(10) Phenanthrene-d10 (I)

16.954min (-0.008) 0.40ng/ul m

response 12597

Ion	Exp%	Act%
188.00	100	100
94.00	10.90	11.75
80.00	12.60	14.25
0.00	0.00	0.00

JU 10/29/19

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN102819\
 Data File : BN008438.D
 Acq On : 28 Oct 2019 13:22
 Operator : JU
 Sample : PB123997BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK97

Manual Integrations
 APPROVED

mohammad
 10/29/2019 3:36:17 PM

Quant Time: Oct 29 11:29:19 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 25 13:14:06 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	1669	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.32	136	8550	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.20	164	5664	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.95	188	12597m	0.40	ng/ul	>0.00
16) Chrysene-d12	21.17	240	10779	0.40	ng/ul	0.00
20) Perylene-d12	23.34	264	12847	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.93	152	3737	0.26	ng/ul	0.00
14) Fluoranthene-d10	19.00	212	11047	0.25	ng/ul	0.00

Target Compounds

Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

2410/29/19