
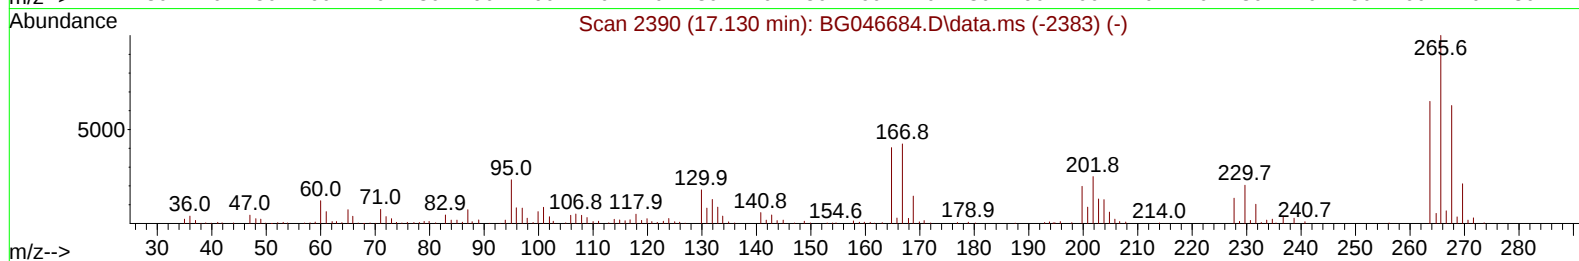
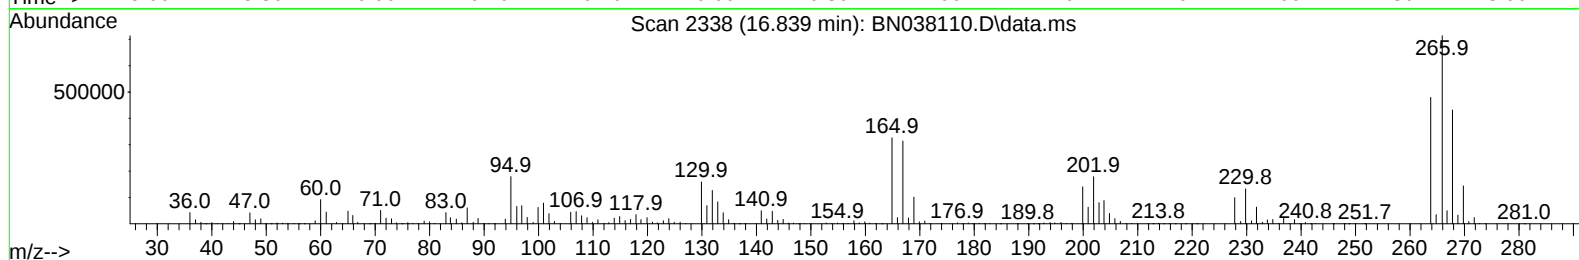


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102825\
Data File : BN038110.D
Acq On : 28 Oct 2025 12:05
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 28 18:06:35 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 28 12:54:48 2025
Response via : Initial Calibration

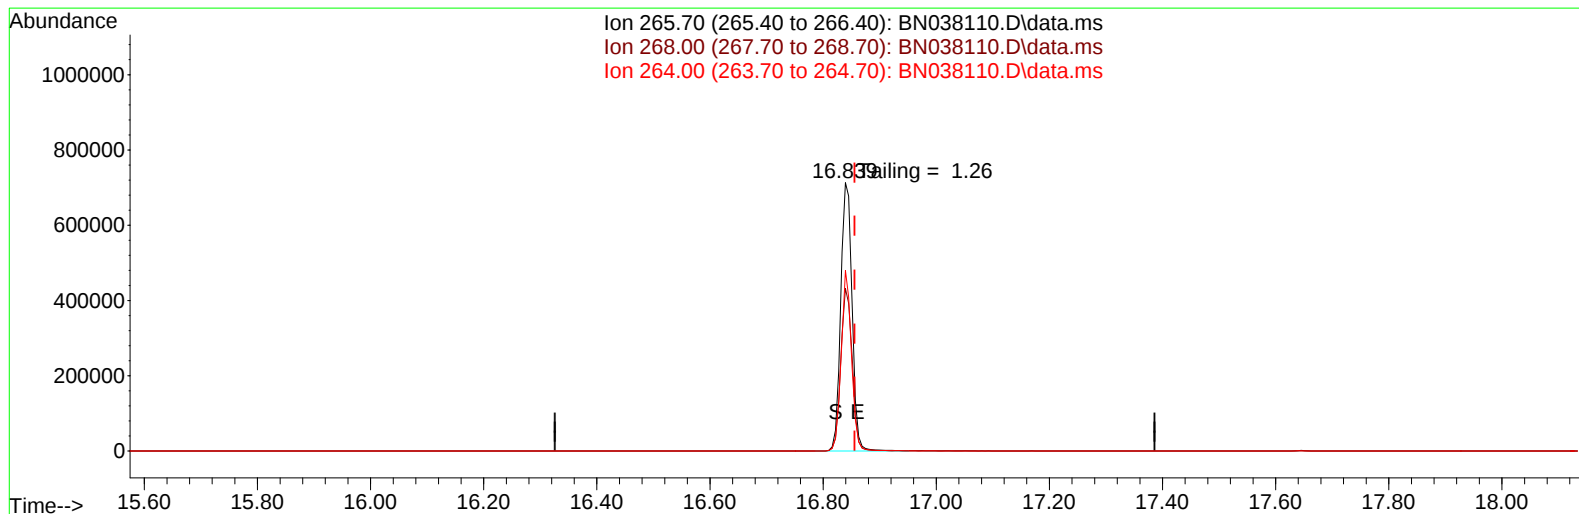

TIC: BN038110.D\data.ms

(70) Pentachlorophenol (C)




16.839min (-0.017) 31764.46 ng

response 993628

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.51
264.00	61.60	67.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102825\
Data File : BN038110.D
Acq On : 28 Oct 2025 12:05
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 28 18:06:35 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 28 12:54:48 2025
Response via : Initial Calibration

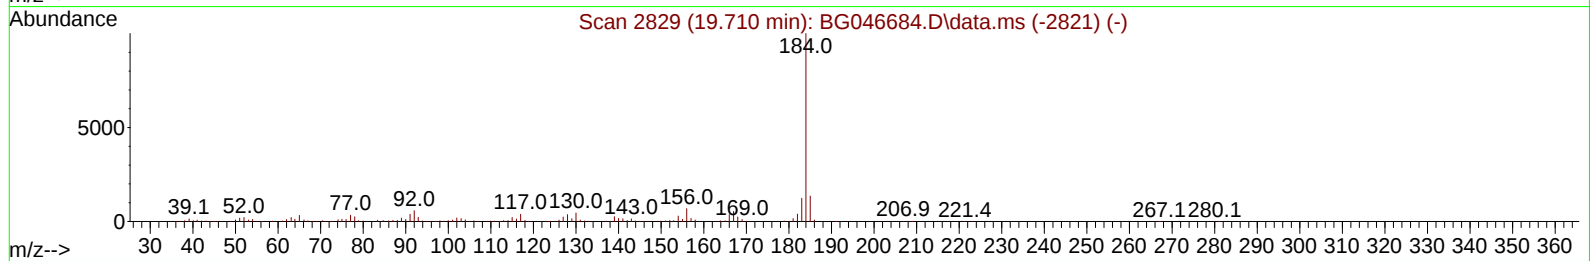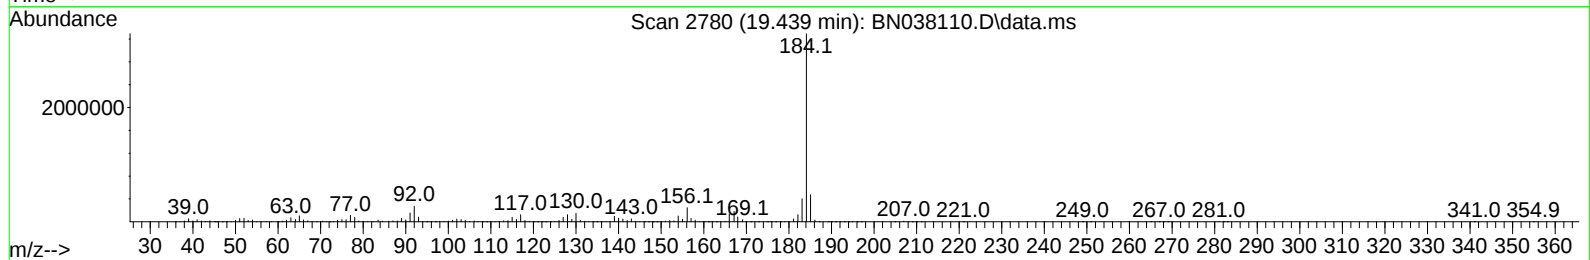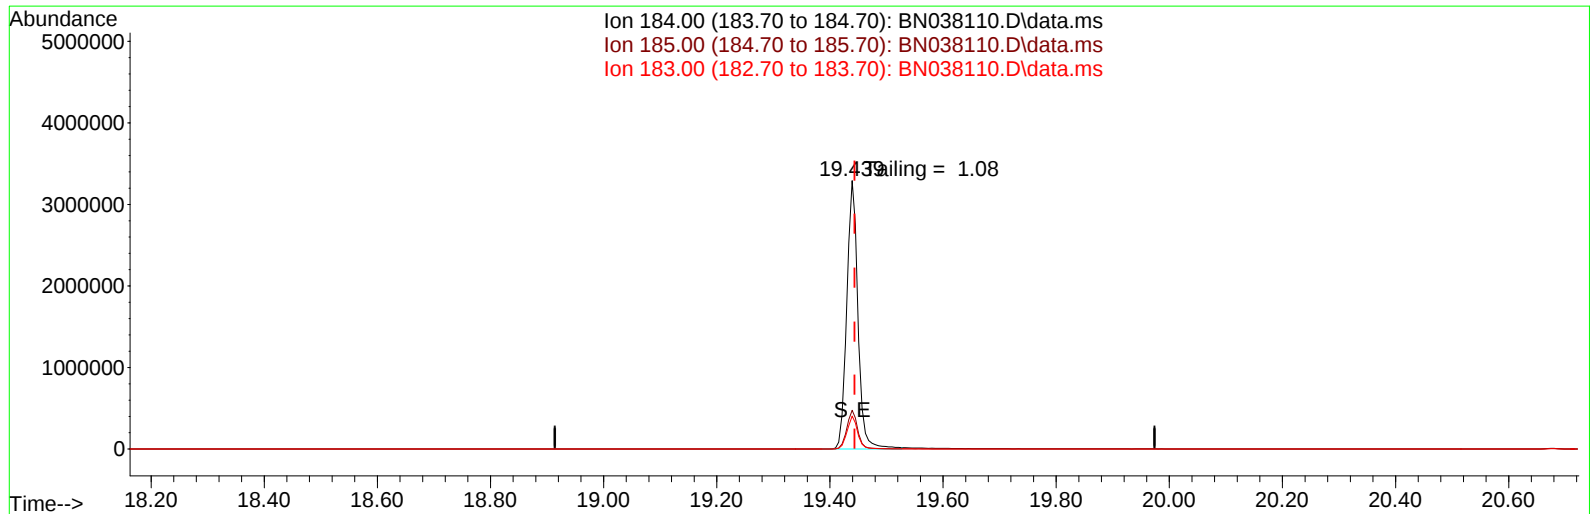

TIC: BN038110.D\data.ms

(77) Benzidine

19.439min (-0.005) 0.00 ng

response 4602519

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.42
183.00	13.20	12.28
0.00	0.00	0.00