

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN102918\
 Data File : BN003330.D
 Acq On : 29 Oct 2018 11:11
 Operator : MJ/SJ
 Sample : PB113752BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 PB113752BL

Quant Time: Oct 30 07:00:39 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN102618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 29 16:15:49 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.86	152	18885	0.40	ng	0.00
7) Naphthalene-d8	10.66	136	80691	0.40	ng	-0.01
13) Acenaphthene-d10	14.49	164	45302	0.40	ng	-0.01
19) Phenanthrene-d10	17.24	188	105335	0.40	ng	0.00
27) Chrysene-d12	21.42	240	115347	0.40	ng	0.00
34) Perylene-d12	23.74	264	110328	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.43	112	20259	0.43	ng	0.00
5) Phenol-d6	7.01	99	25567	0.43	ng	0.00
8) Nitrobenzene-d5	9.02	82	16209	0.46	ng	0.00
11) 2-Methylnaphthalene-d10	12.25	152	45338	0.35	ng	0.00
14) 2,4,6-Tribromophenol	15.98	330	5669	0.31	ng	0.00
15) 2-Fluorobiphenyl	13.12	172	68676	0.35	ng	-0.01
25) Fluoranthene-d10	19.26	212	112555	0.37	ng	0.00
29) Terphenyl-d14	19.86	244	84221	0.31	ng	0.00


Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN102918\
Data File : BN003330.D
Acq On : 29 Oct 2018 11:11
Operator : MJ/SJ
Sample : PB113752BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB113752BL

Quant Time: Oct 30 07:00:39 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN102618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 29 16:15:49 2018
Response via : Initial Calibration

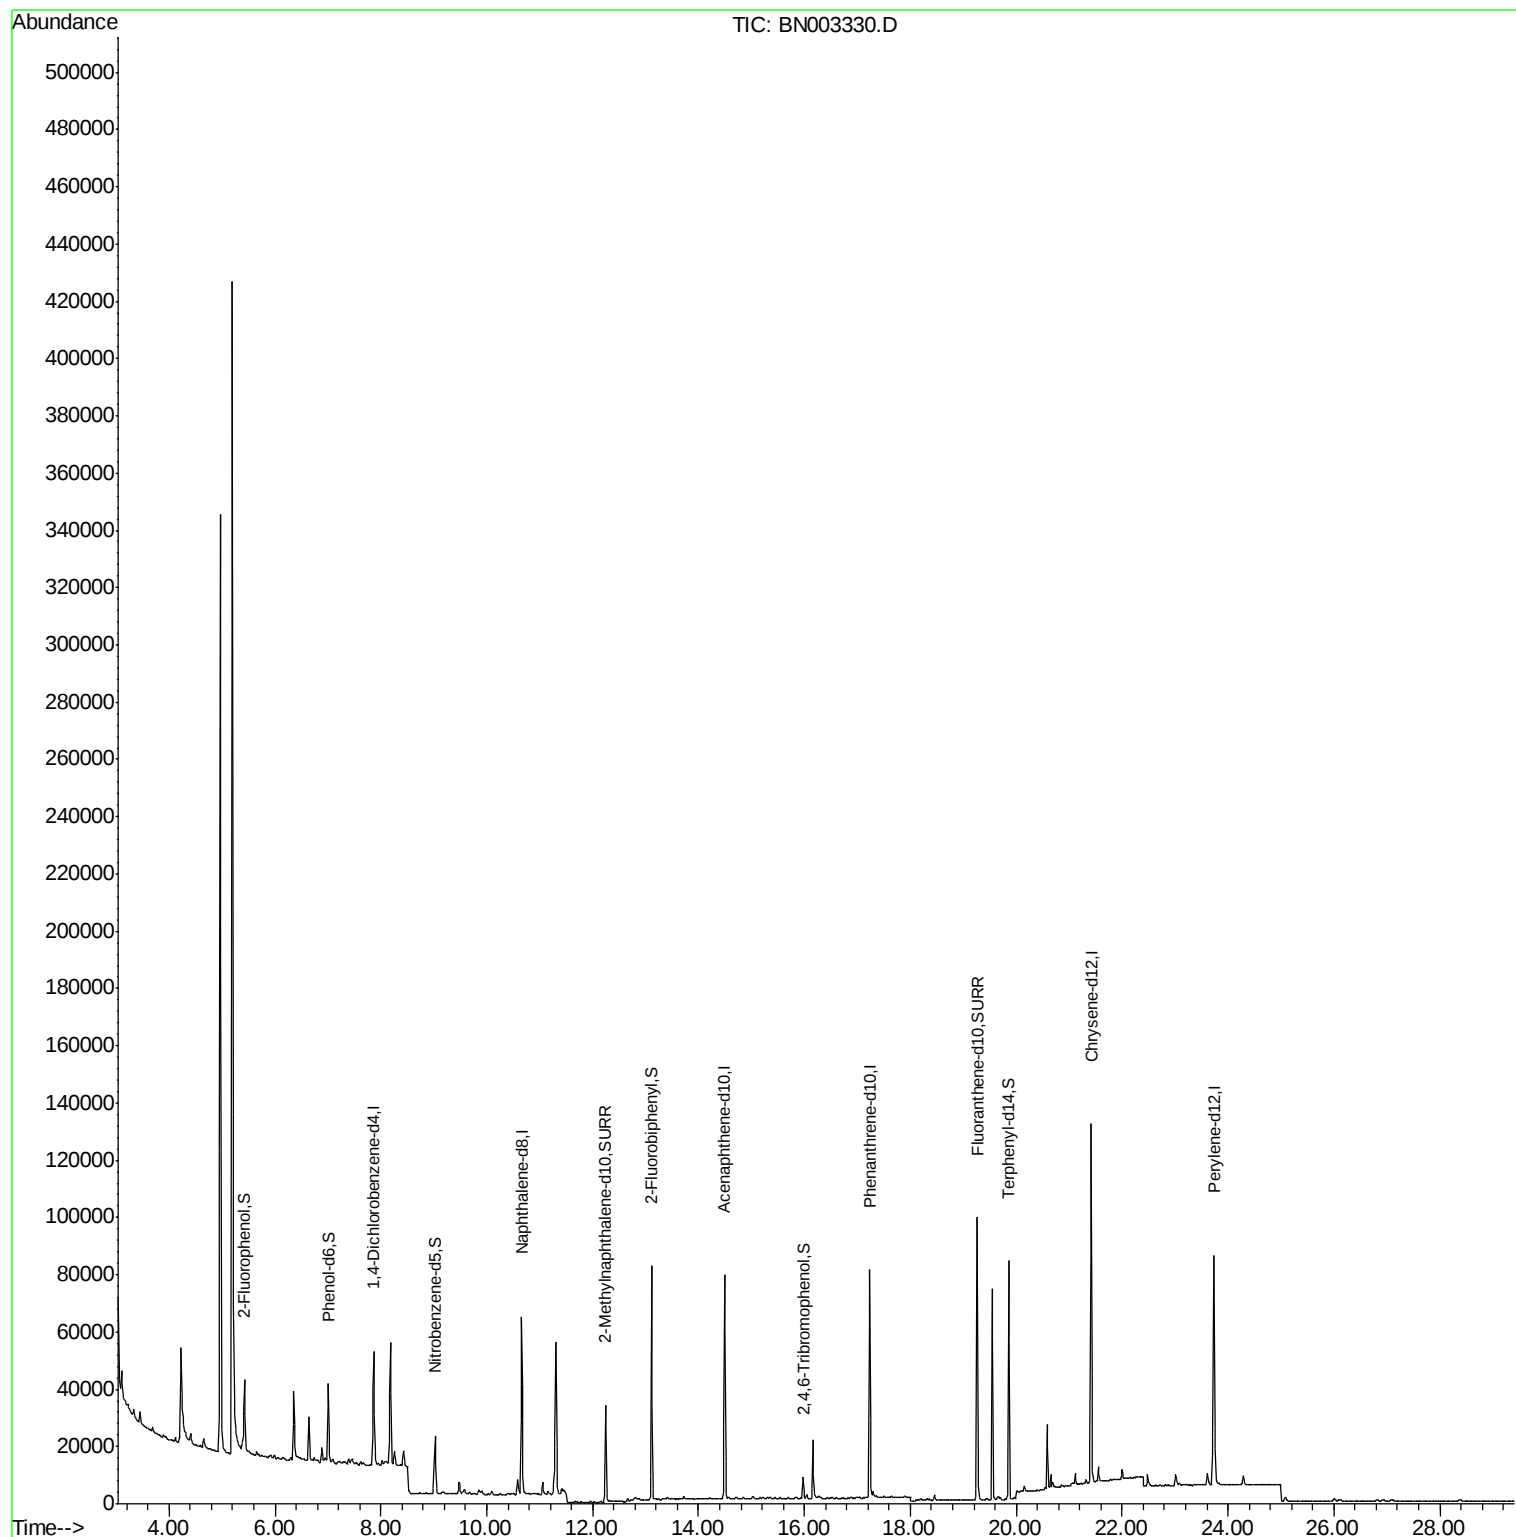




#1




1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.86 min Scan# 600
Delta R.T. -0.01 min
Lab File: BN003330.D
Acq: 29 Oct 2018 11:11

Instrument :
BNA_N
ClientSampleId :
PB113752BL

Tot Ion:152 Resp: 18885
Ion Ratio Lower Upper
152 100
150 155.8 124.6 187.0
115 58.1 46.4 69.6

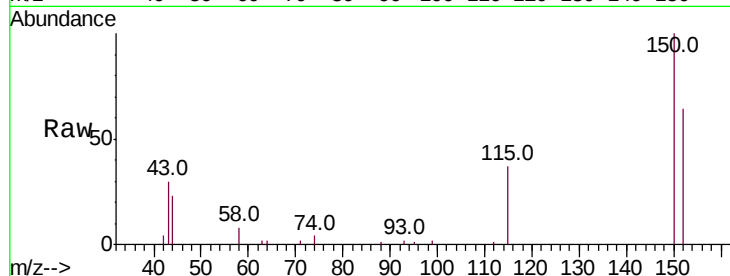


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

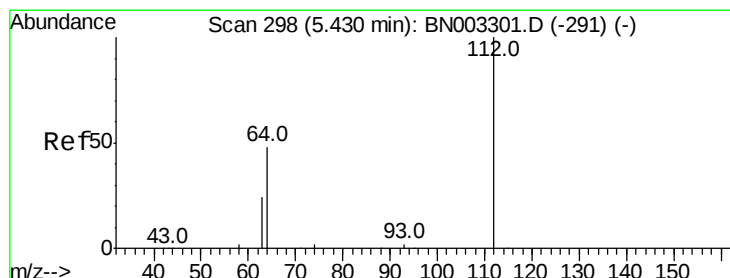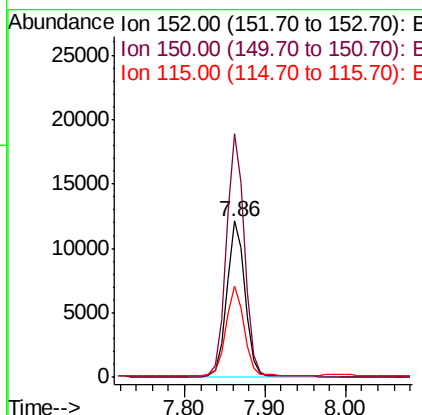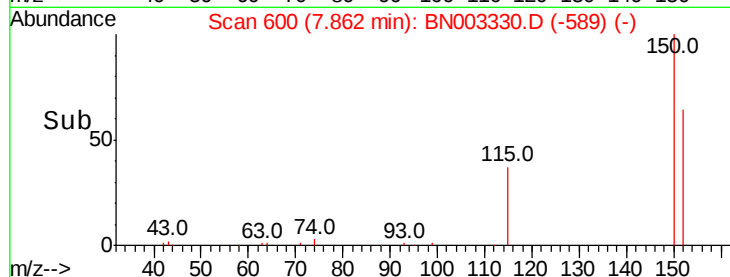



#4


2-Fluorophenol
Concen: 0.433 ng
RT: 5.43 min Scan# 298
Delta R.T. -0.00 min
Lab File: BN003330.D
Acq: 29 Oct 2018 11:11

Tgt Ion:112 Resp: 20259
Ion Ratio Lower Upper
112 100
64 54.3 44.3 66.5
63 26.9 22.4 33.6

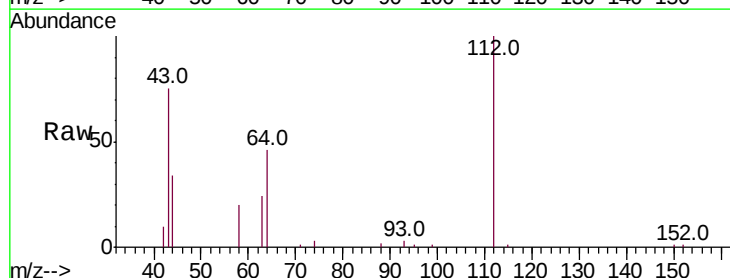

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BNC
Ion 63.00 (62.70 to 63.70): BNC

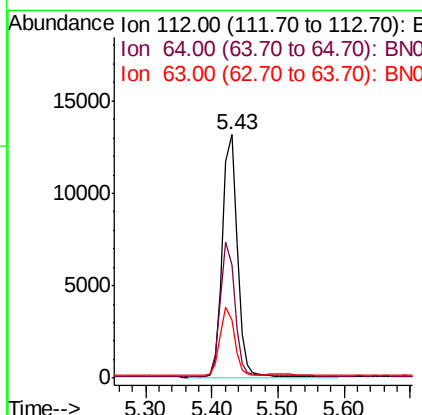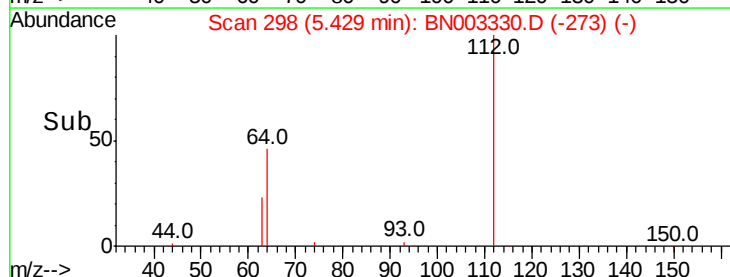

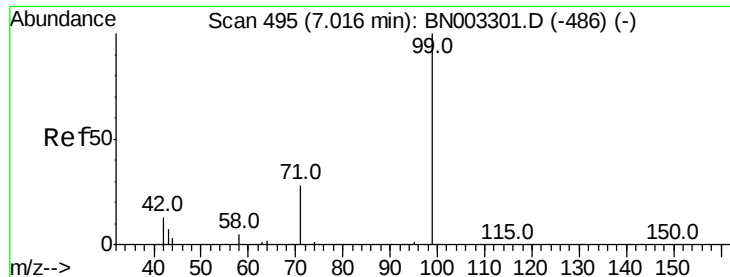

#5

Phenol-d6

Concen: 0.433 ng

RT: 7.01 min Scan# 494

Delta R.T. -0.01 min

Lab File: BN003330.D

Acq: 29 Oct 2018 11:11

Instrument :


BNA_N

ClientSampleId :

PB113752BL

Tot Ion: 99 Resp: 25567

Ion	Ratio	Lower	Upper
99	100		
42	17.6	14.8	22.2
71	30.0	24.8	37.2



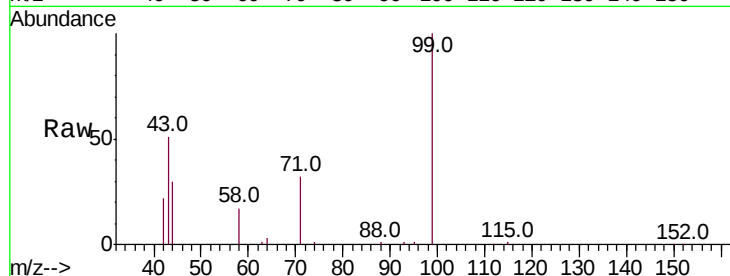


Abundance

Ion 99.00 (98.70 to 99.70): BN003330.D (-486) (-)

Ion 42.00 (41.70 to 42.70): BN003330.D (-486) (-)

Ion 71.00 (70.70 to 71.70): BN003330.D (-486) (-)

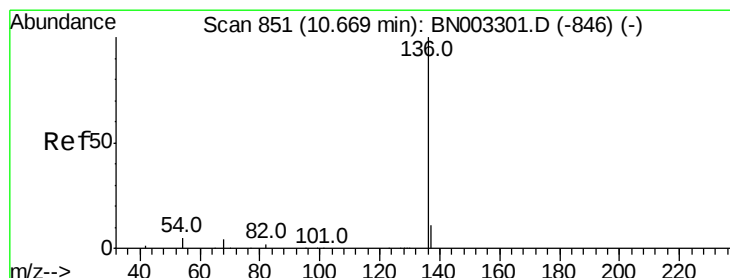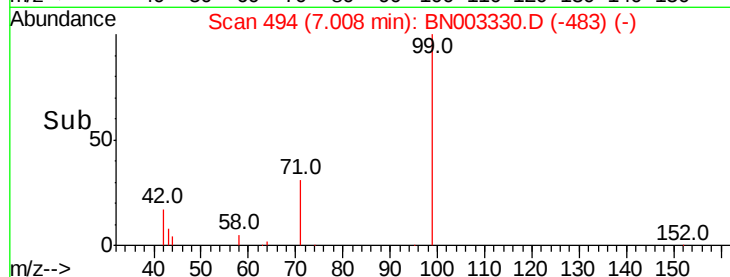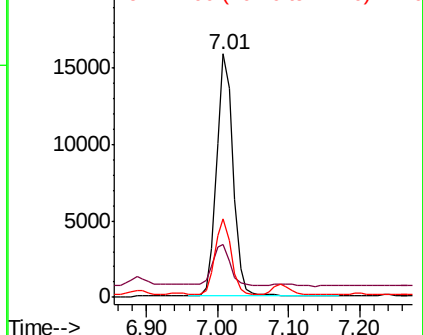

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.66 min Scan# 850


Delta R.T. -0.01 min

Lab File: BN003330.D

Acq: 29 Oct 2018 11:11

Tgt Ion: 136 Resp: 80691

Ion	Ratio	Lower	Upper
136	100		
137	11.0	9.0	13.4
54	7.1	4.1	6.1#
68	6.1	3.5	5.3#

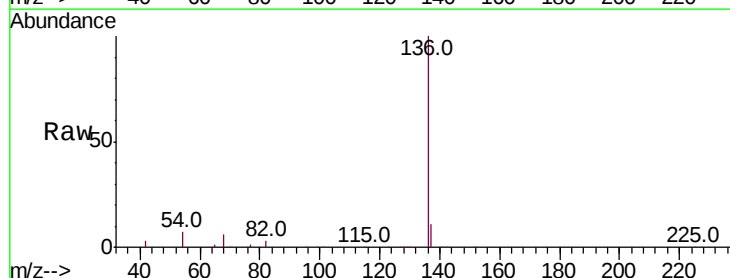



Abundance


Ion 136.00 (135.70 to 136.70): BN003330.D (-846) (-)

Ion 137.00 (136.70 to 137.70): BN003330.D (-846) (-)

Ion 54.00 (53.70 to 54.70): BN003330.D (-846) (-)

Ion 68.00 (67.70 to 68.70): BN003330.D (-846) (-)

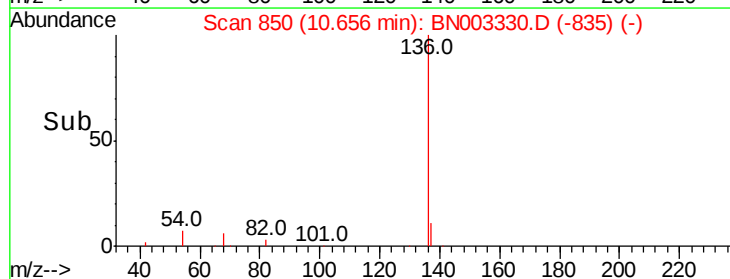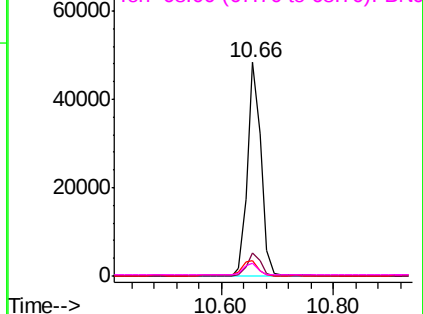

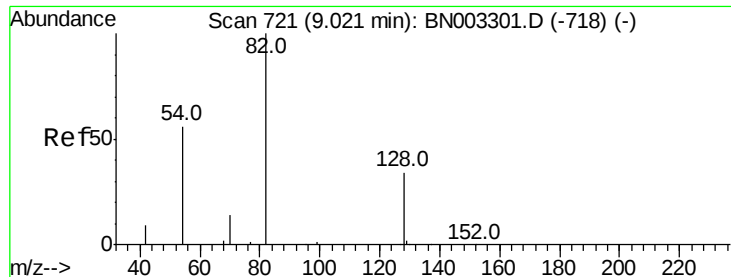

#8

Nitrobenzene-d5

Concen: 0.459 ng

RT: 9.02 min Scan# 721

Delta R.T. -0.00 min

Lab File: BN003330.D

Acq: 29 Oct 2018 11:11

Instrument :

BNA_N

ClientSampleId :

PB113752BL


Tot Ion: 82 Resp: 16209

Ion Ratio Lower Upper

82 100

128 44.5 28.9 43.3#




54 48.7 46.1 69.1

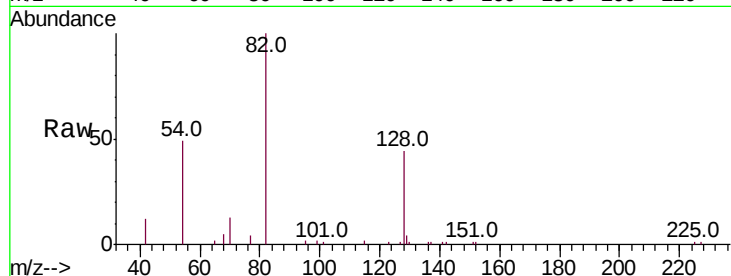

Abundance Ion 82.00 (81.70 to 82.70): BN003330.D (-718) (-)

Ion 128.00 (127.70 to 128.70): BN003330.D (-718) (-)

Ion 54.00 (53.70 to 54.70): BN003330.D (-718) (-)

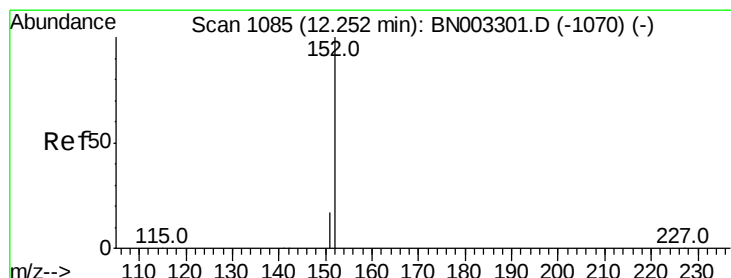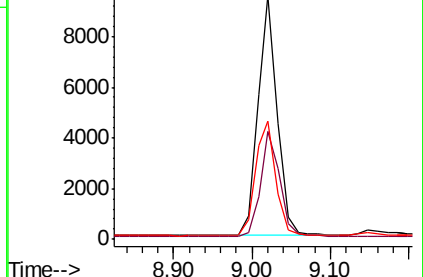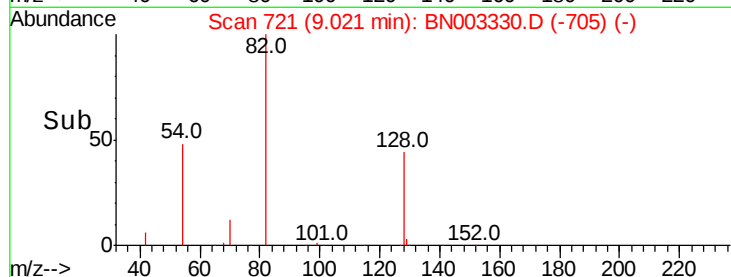

#11

2-Methylnaphthalene-d10

Concen: 0.345 ng

RT: 12.25 min Scan# 1084

Delta R.T. -0.00 min

Lab File: BN003330.D


Acq: 29 Oct 2018 11:11

Tgt Ion: 152 Resp: 45338

Ion Ratio Lower Upper



152 100


151 19.2 15.1 22.7

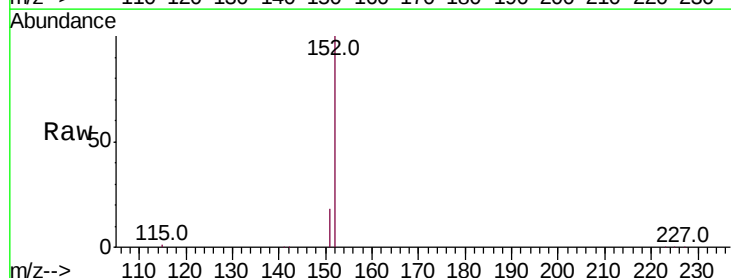

Abundance Ion 152.00 (151.70 to 152.70): BN003330.D (-1040) (-)

Ion 151.00 (150.70 to 151.70): BN003330.D (-1040) (-)

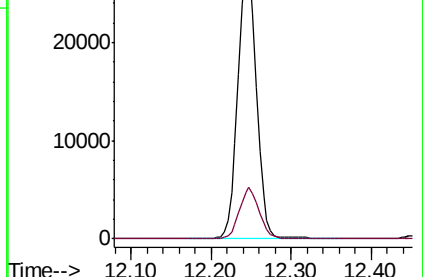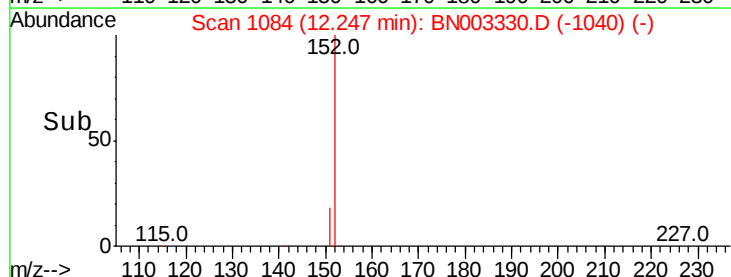

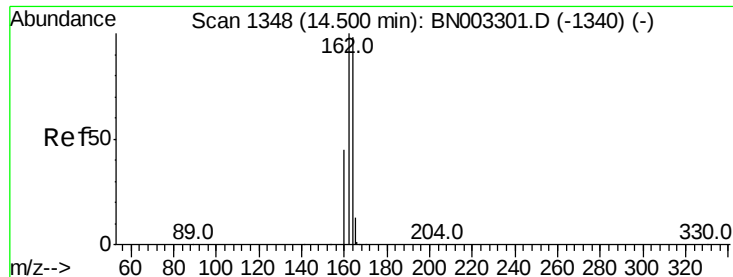

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.49 min Scan# 1347

Delta R.T. -0.01 min

Lab File: BN003330.D

Acq: 29 Oct 2018 11:11

Instrument :

BNA_N

ClientSampleId :

PB113752BL


Tot Ion:164 Resp: 45302

Ion Ratio Lower Upper

164 100

162 104.1 81.8 122.6




160 48.5 37.2 55.8

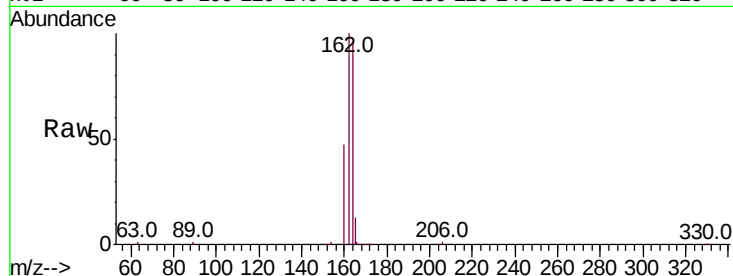

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

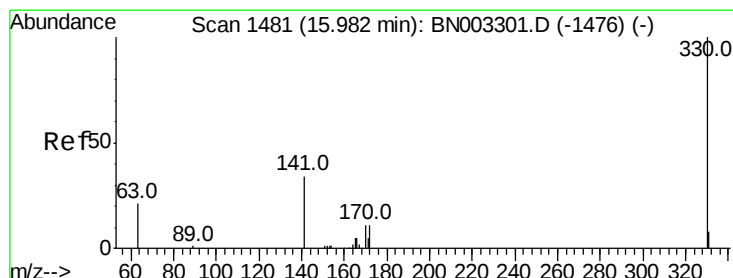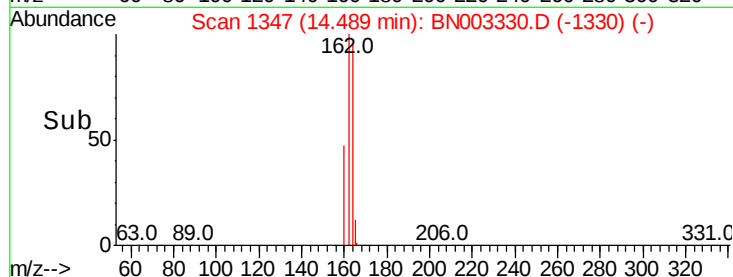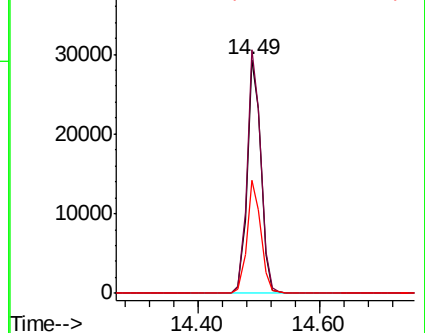

#14

2,4,6-Tribromophenol

Concen: 0.314 ng

RT: 15.98 min Scan# 1481

Delta R.T. -0.00 min

Lab File: BN003330.D

Acq: 29 Oct 2018 11:11


Tgt Ion:330 Resp: 5669

Ion Ratio Lower Upper

330 100

332 0.0 0.0 0.0



141 34.8 28.3 42.5

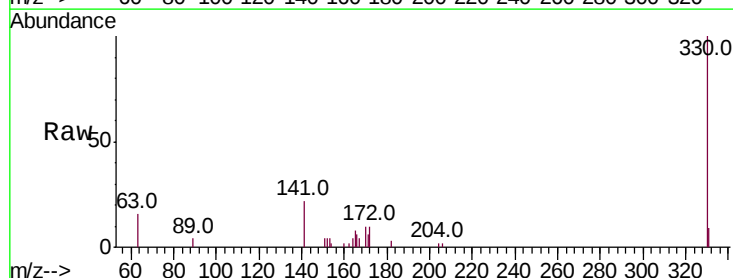


Abundance Ion 330.00 (329.70 to 330.70): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

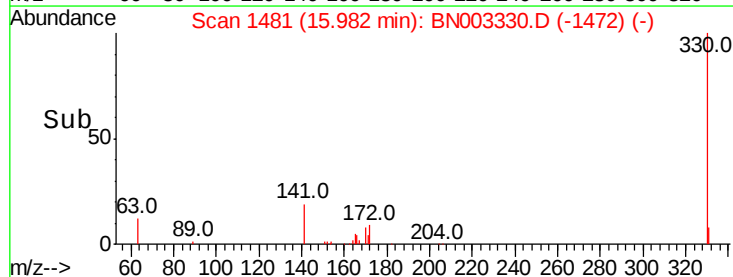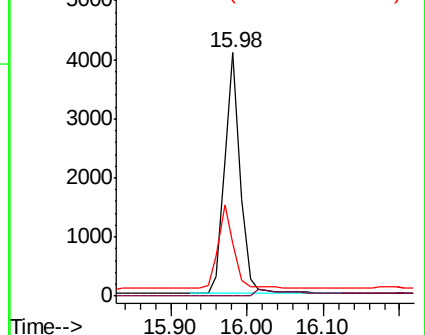

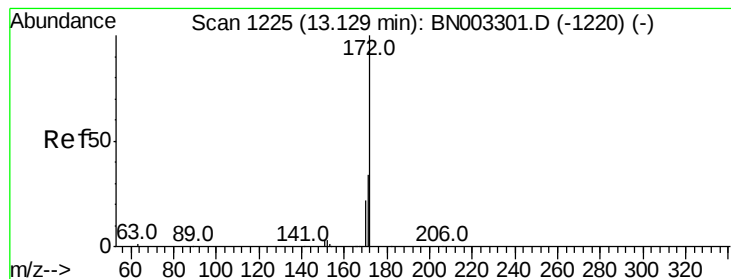

#15

2-Fluorobiphenyl

Concen: 0.352 ng

RT: 13.12 min Scan# 1224

Delta R.T. -0.01 min

Lab File: BN003330.D

Acq: 29 Oct 2018 11:11

Instrument :


BNA_N

ClientSampleId :

PB113752BL

Tot Ion:172 Resp: 68676




Ion	Ratio	Lower	Upper
172	100		
171	34.8	27.1	40.7
170	22.7	17.4	26.0

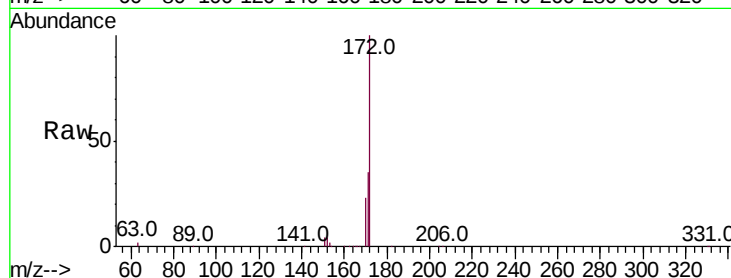

Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

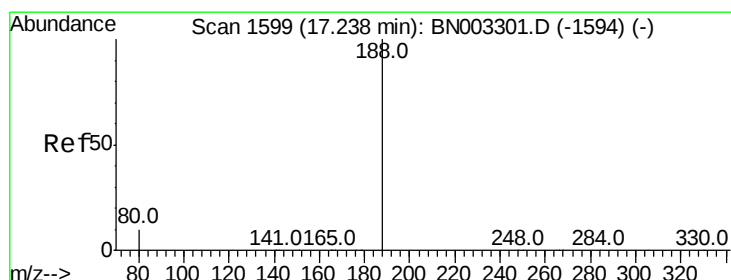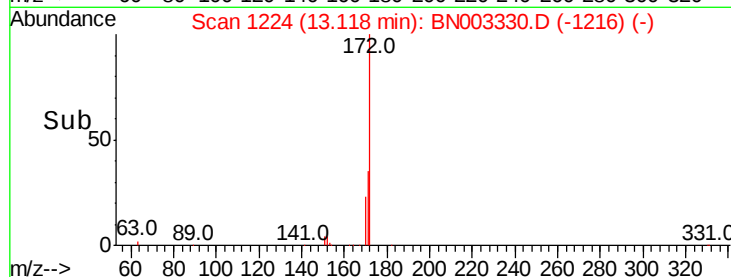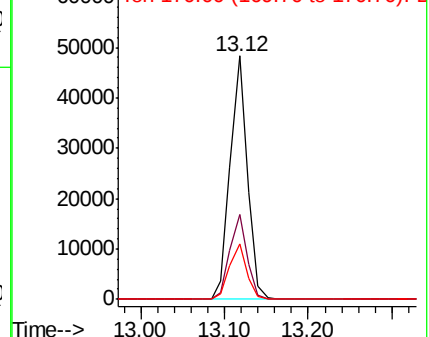

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.24 min Scan# 1599


Delta R.T. -0.00 min

Lab File: BN003330.D

Acq: 29 Oct 2018 11:11

Tgt Ion:188 Resp: 105335



Ion	Ratio	Lower	Upper
188	100		
94	0.0	0.0	0.0
80	7.7	8.6	12.8

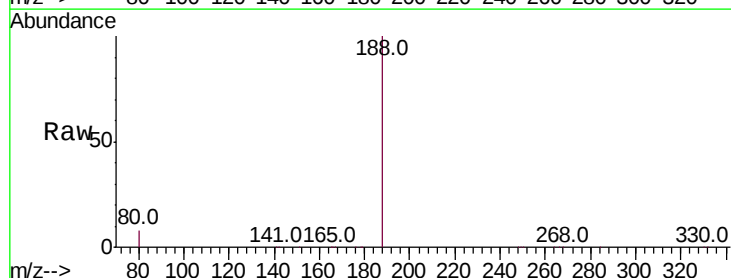


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BNC

Ion 80.00 (79.70 to 80.70): BNC

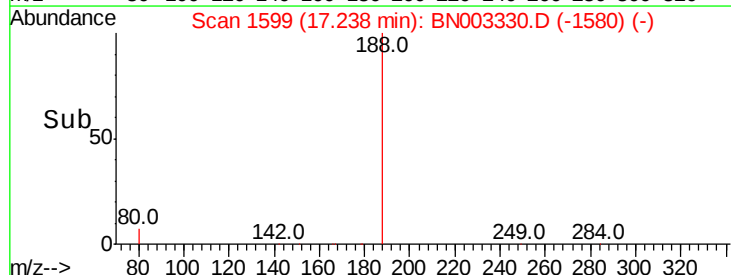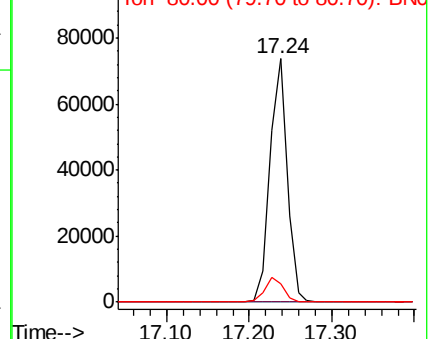

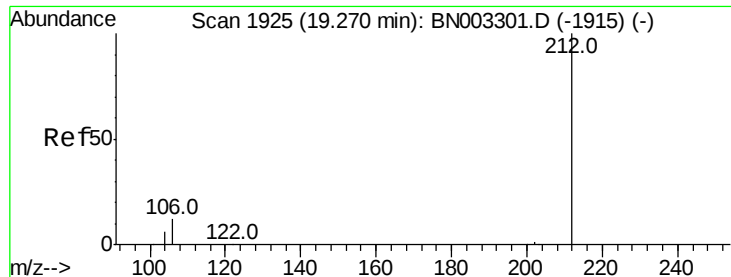

#25

Fluoranthene-d10

Concen: 0.367 ng

RT: 19.26 min Scan# 1924

Delta R.T. -0.01 min

Lab File: BN003330.D

Acq: 29 Oct 2018 11:11

Instrument :

BNA_N

ClientSampleId :

PB113752BL


Tot Ion:212 Resp: 112555

Ion Ratio Lower Upper

212 100

106 12.8 10.3 15.5




104 7.0 5.6 8.4

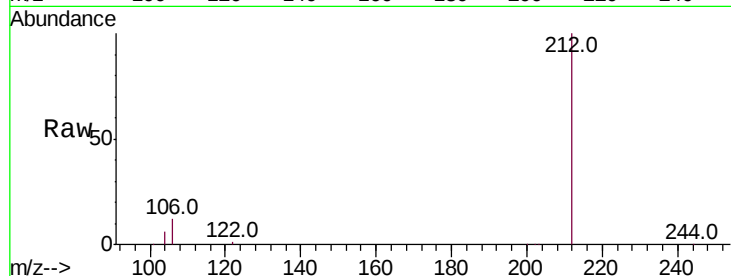

Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

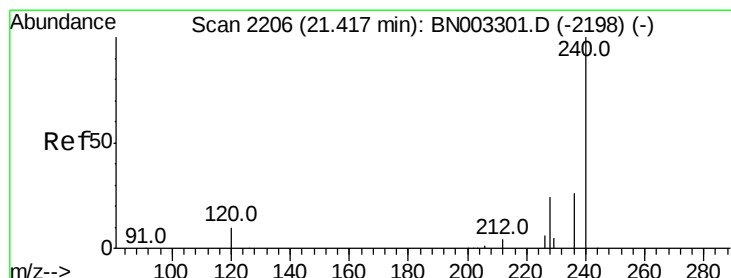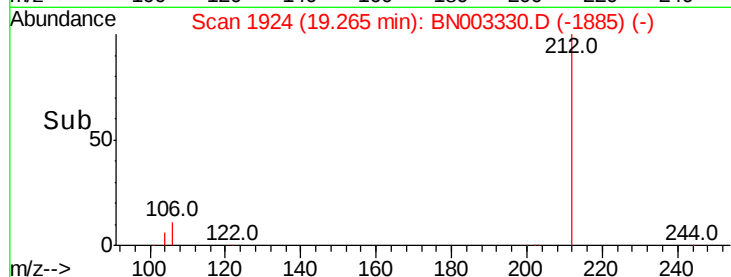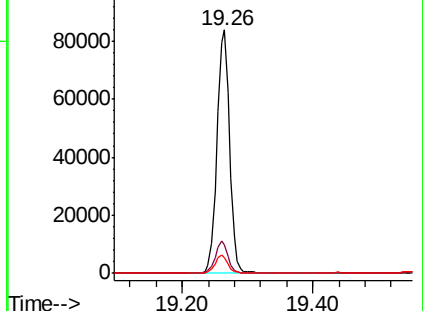

#27

Chrysene-d12

Concen: 0.400 ng

RT: 21.42 min Scan# 2206

Delta R.T. -0.00 min

Lab File: BN003330.D

Acq: 29 Oct 2018 11:11


Tgt Ion:240 Resp: 115347

Ion Ratio Lower Upper

240 100

120 6.9 9.3 13.9#



236 25.8 21.0 31.4

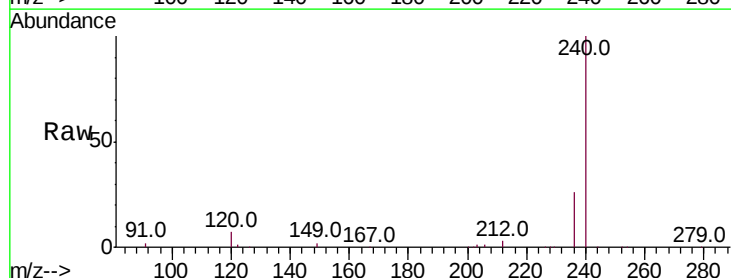


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

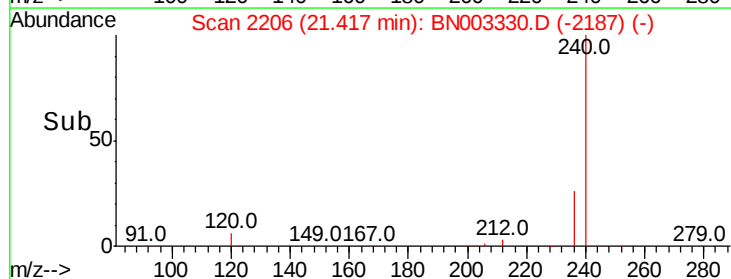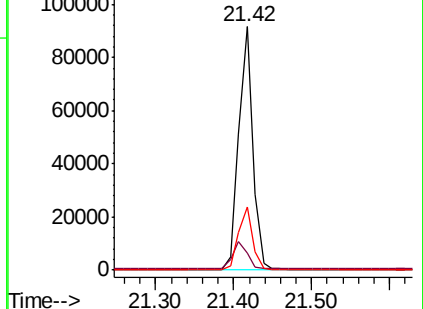

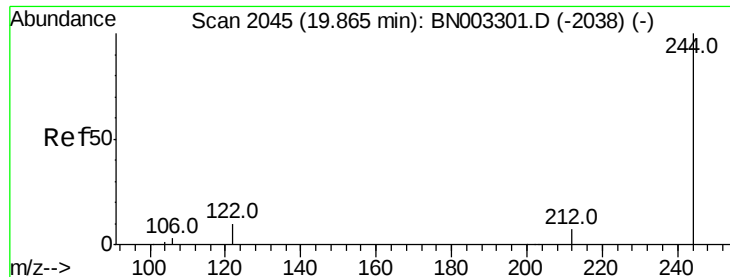

#29

Terphenyl-d14

Concen: 0.314 ng

RT: 19.86 min Scan# 2043

Delta R.T. -0.01 min

Lab File: BN003330.D

Acq: 29 Oct 2018 11:11

Instrument :

BNA_N

ClientSampleId :

PB113752BL


Tot Ion:244 Resp: 84221

Ion Ratio Lower Upper

244 100

212 7.0 5.6 8.4




122 11.8 8.5 12.7

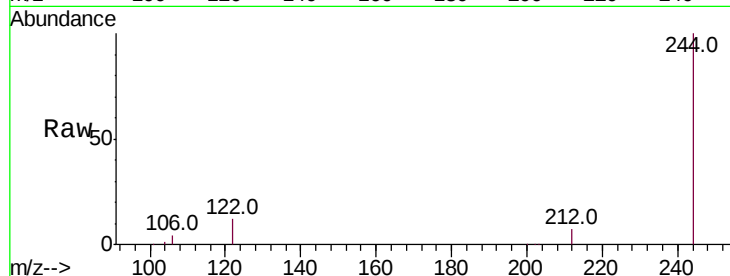

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

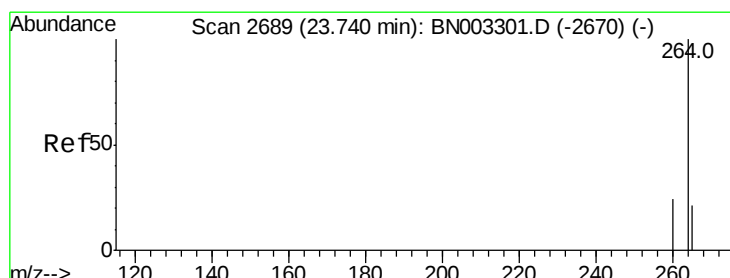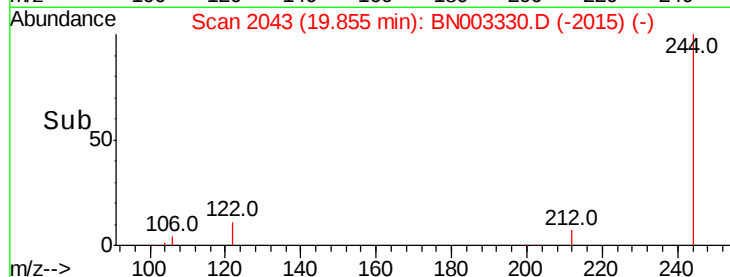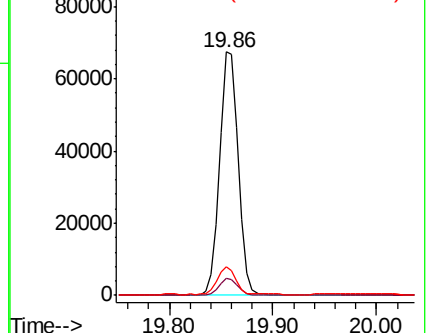

#34

Perylene-d12

Concen: 0.400 ng

RT: 23.74 min Scan# 2688

Delta R.T. -0.00 min

Lab File: BN003330.D

Acq: 29 Oct 2018 11:11


Tgt Ion:264 Resp: 110328

Ion Ratio Lower Upper

264 100

260 24.0 19.1 28.7

265 28.3 26.4 39.6

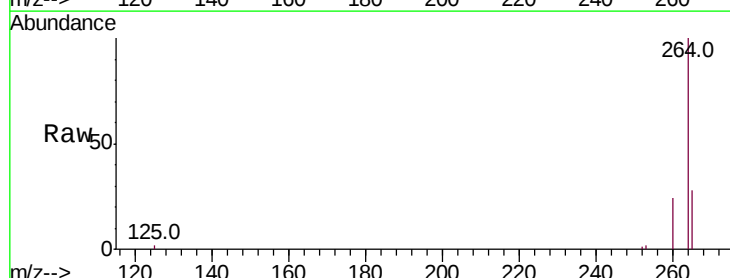

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

