
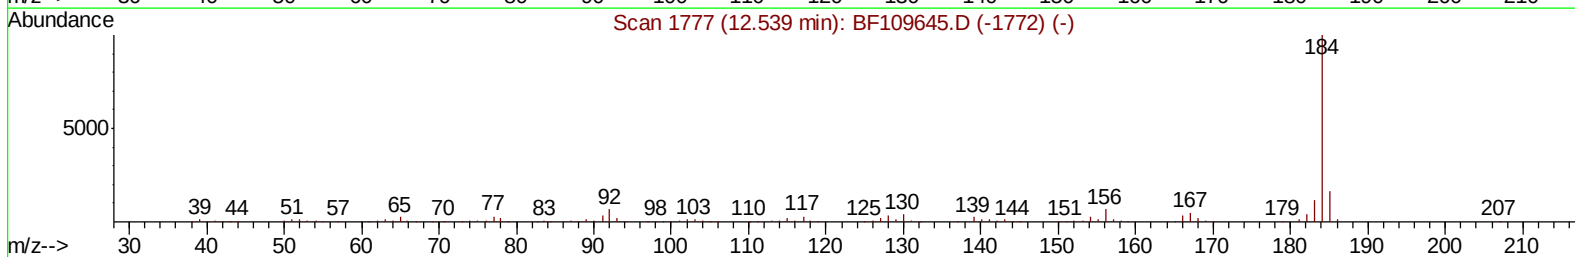
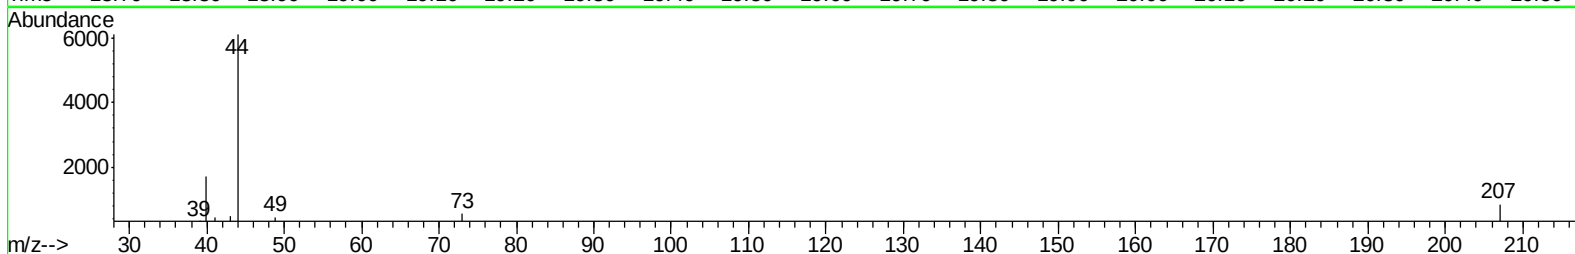


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN102918\
 Data File : BN003328.D
 Acq On : 29 Oct 2018 09:23
 Operator : MJ/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 30 08:43:57 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 08 16:02:11 2018
 Response via : Initial Calibration

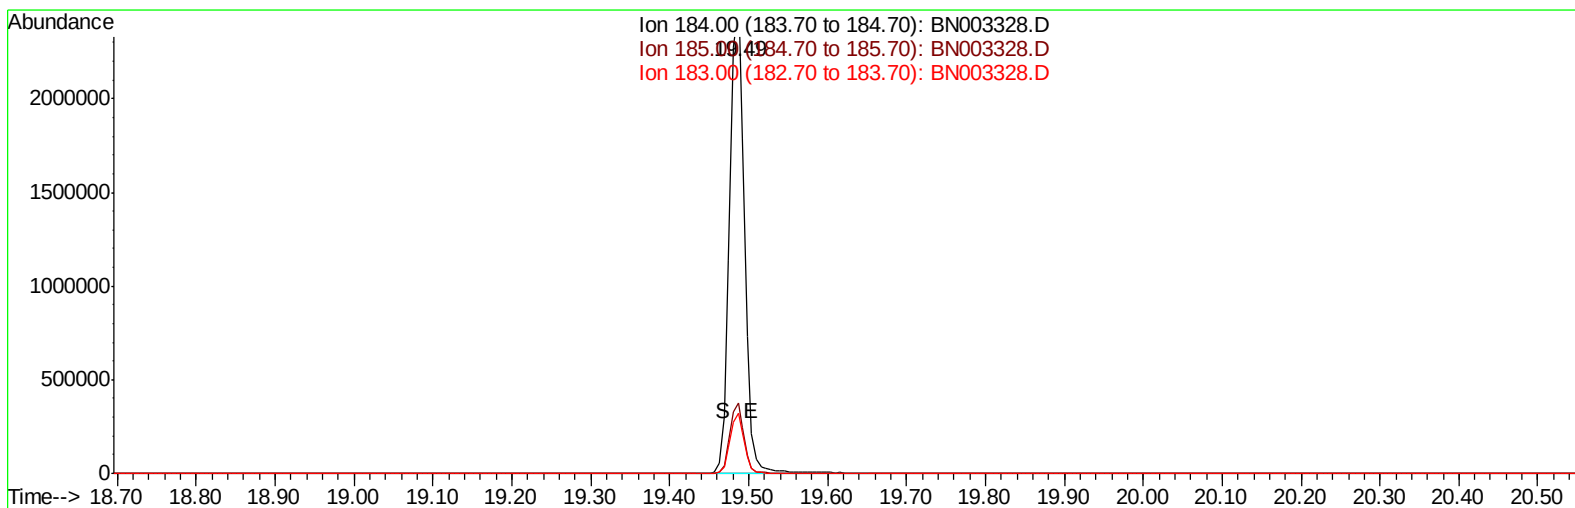

TIC: BN003328.D

(76) Benzidine




12.539min (-12.539) 0.00ng

response 0

Ion	Exp%	Act%
184.00	100	0.00
185.00	16.80	0.00#
183.00	11.80	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN102918\
 Data File : BN003328.D
 Acq On : 29 Oct 2018 09:23
 Operator : MJ/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 30 08:43:57 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 08 16:02:11 2018
 Response via : Initial Calibration

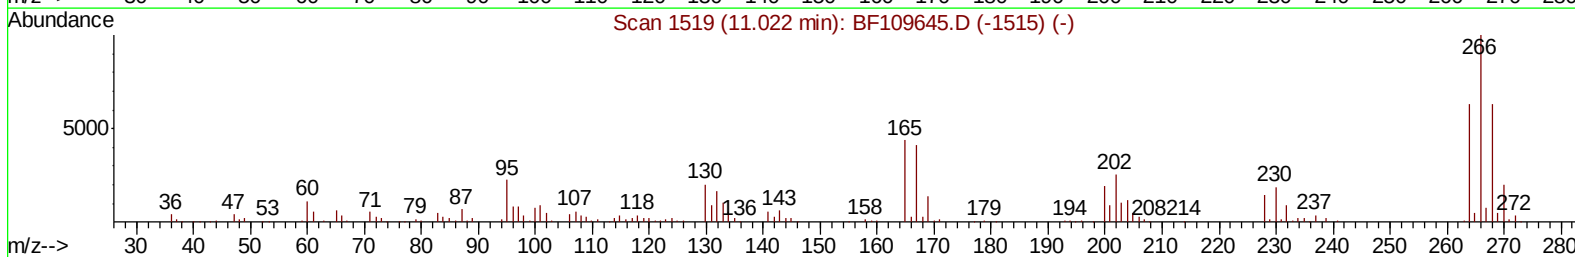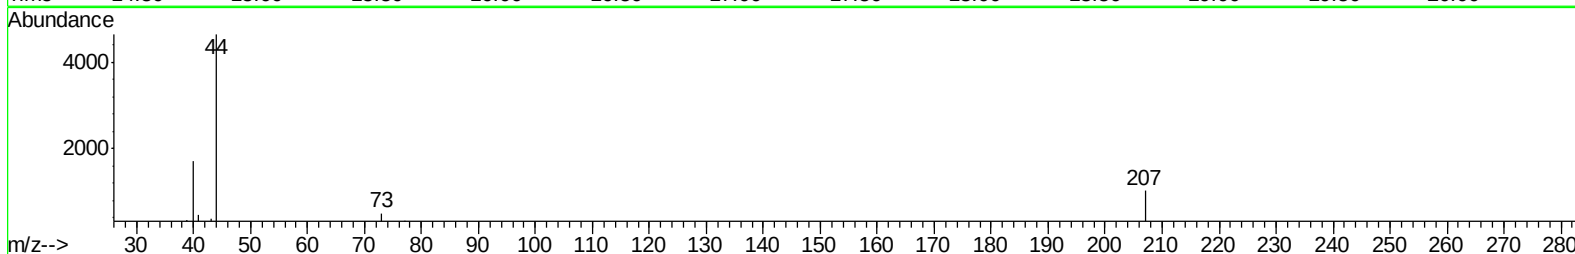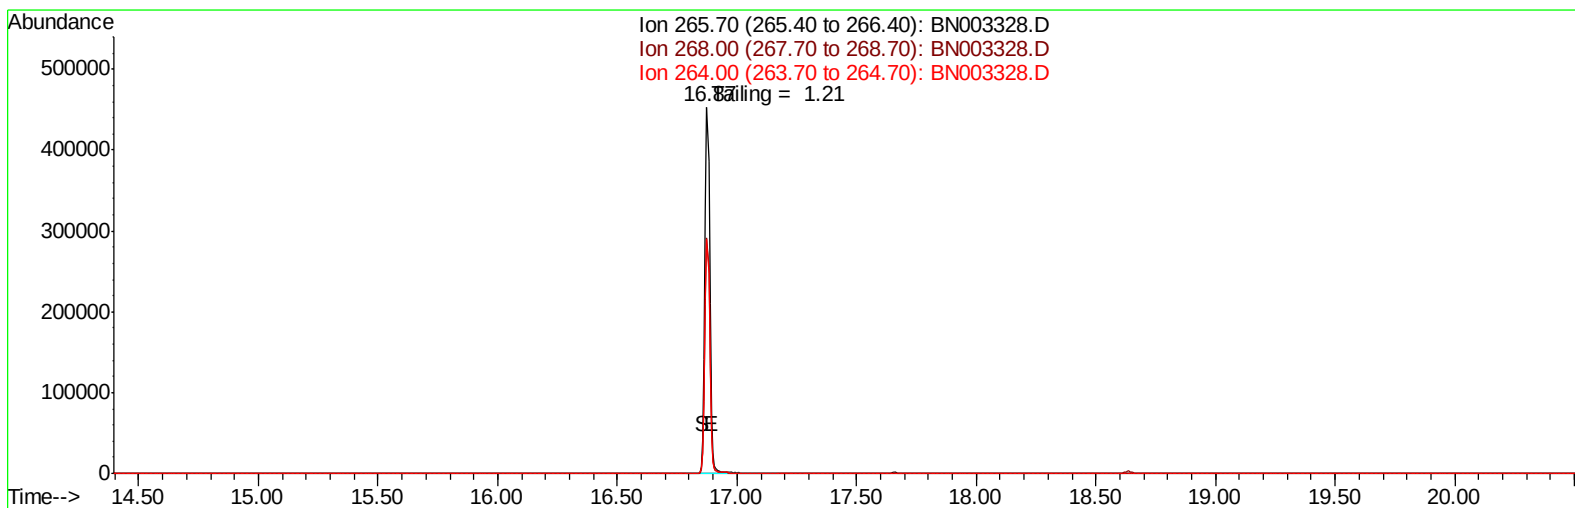

TIC: BN003328.D

(69) Pentachlorophenol (C)

11.022min (-11.022) 0.00ng

response 0

Ion	Exp%	Act%
265.70	100	0.00
268.00	63.20	0.00#
264.00	63.20	0.00#
0.00	0.00	0.00