


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102918\
 Data File : BN003328.D
 Acq On : 29 Oct 2018 09:23
 Operator : MJ/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN102618.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 29 16:15:49 2018

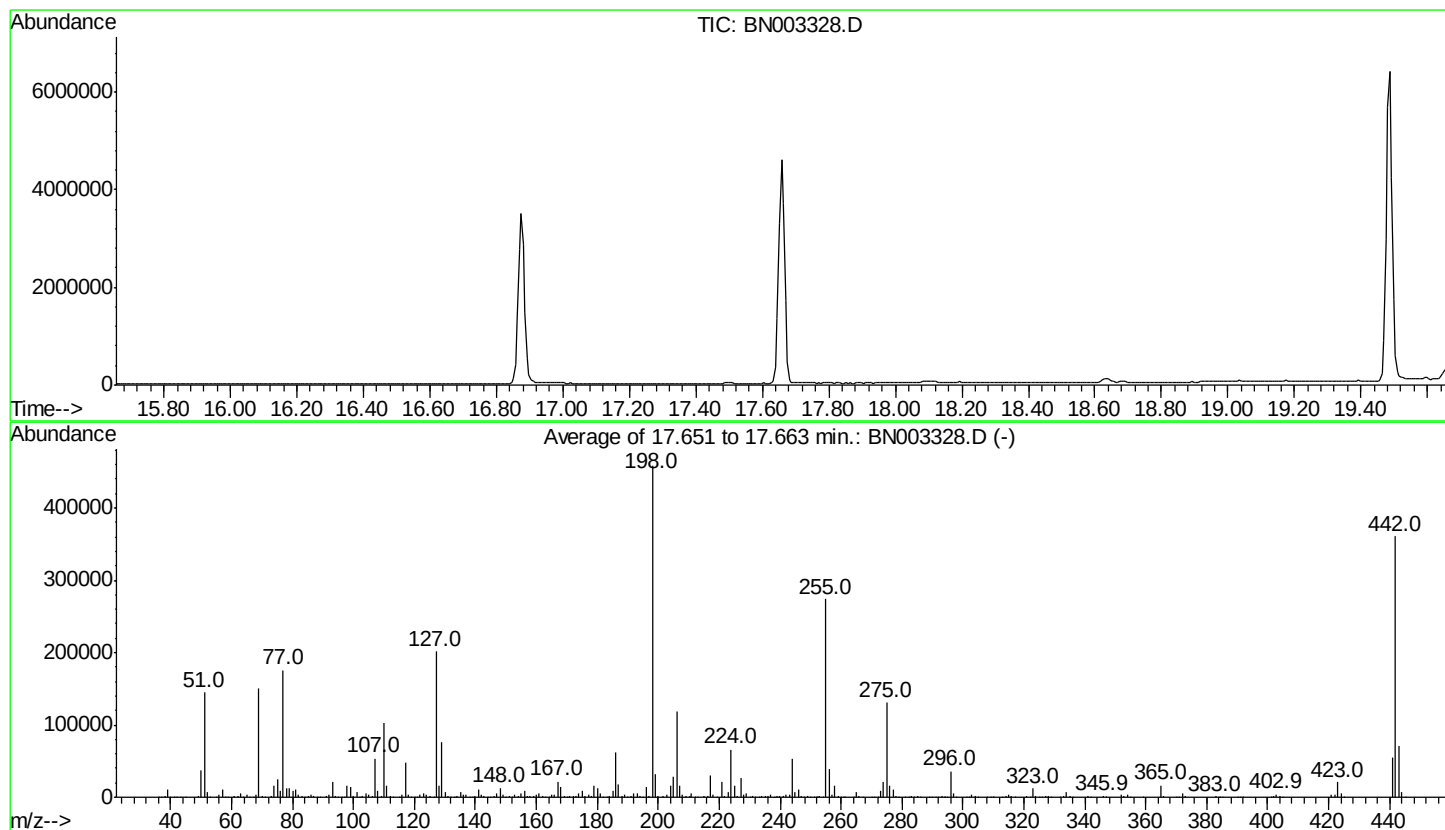

AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2486

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.6	145085	PASS
68	69	0.00	2	1.9	2792	PASS
69	198	0.00	100	32.6	149665	PASS
70	69	0.00	2	0.7	974	PASS
127	198	10	80	43.9	201130	PASS
197	198	0.00	2	0.6	2584	PASS
198	198	100	100	100.0	458432	PASS
199	198	5	9	6.8	31322	PASS
275	198	10	60	28.5	130634	PASS
365	198	1	100	3.5	16100	PASS
441	198	0.01	100	12.0	54837	PASS
442	198	50	100	78.6	360256	PASS
443	442	15	24	19.4	69973	PASS