

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102921\
 Data File : BN017182.D
 Acq On : 29 Oct 2021 15:33
 Operator : CG/JU
 Sample : SSTDICC0.2
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.2

Quant Time: Oct 29 17:24:01 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN102921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 29 17:22:00 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.560	152	31735	0.400	ng	0.00
7) Naphthalene-d8	10.332	136	142939	0.400	ng	0.00
13) Acenaphthene-d10	14.194	164	73172	0.400	ng	0.00
19) Phenanthrene-d10	16.946	188	133238	0.400	ng	0.00
29) Chrysene-d12	21.165	240	122711	0.400	ng	0.00
35) Perylene-d12	23.373	264	128068	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.172	112	14614	0.219	ng	0.00
5) Phenol-d6	6.749	99	15408	0.202	ng	0.00
8) Nitrobenzene-d5	8.709	82	14940	0.161	ng	0.00
11) 2-Methylnaphthalene-d10	11.928	152	42048	0.207	ng	0.00
14) 2,4,6-Tribromophenol	15.704	330	4042	0.136	ng	0.00
15) 2-Fluorobiphenyl	12.823	172	59195	0.216	ng	0.00
27) Fluoranthene-d10	18.994	212	65519	0.196	ng	0.00
31) Terphenyl-d14	19.610	244	55047	0.203	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.162	88	3892	0.189	ng	# 15
3) n-Nitrosodimethylamine	3.494	42	5537	0.225	ng	100
6) bis(2-Chloroethyl)ether	7.007	93	17991	0.205	ng	100
9) Naphthalene	10.382	128	82029	0.221	ng	100
10) Hexachlorobutadiene	10.674	225	14791	0.201	ng	# 100
12) 2-Methylnaphthalene	12.004	142	50496	0.211	ng	99
16) Acenaphthylene	13.915	152	54747	0.185	ng	100
17) Acenaphthene	14.257	154	42957	0.212	ng	100
18) Fluorene	15.259	166	49607	0.203	ng	99
20) 4,6-Dinitro-2-methylph...	15.348	198	1899	0.135	ng	# 91
21) 4-Bromophenyl-phenylether	16.155	248	14621	0.188	ng	100
22) Hexachlorobenzene	16.264	284	16927	0.190	ng	99
23) Atrazine	16.434	200	8553	0.166	ng	99
24) Pentachlorophenol	16.617	266	3782	0.154	ng	99
25) Phenanthrene	16.994	178	79104	0.209	ng	100
26) Anthracene	17.079	178	58310	0.182	ng	99
28) Fluoranthene	19.024	202	82290	0.200	ng	100
30) Pyrene	19.392	202	81190	0.210	ng	100
32) Benzo(a)anthracene	21.144	228	70015	0.193	ng	100
33) Chrysene	21.197	228	84713	0.212	ng	100
34) Bis(2-ethylhexyl)phtha...	21.101	149	24367	0.155	ng	100
36) Indeno(1,2,3-cd)pyrene	25.597	276	96537	0.221	ng	100
37) Benzo(b)fluoranthene	22.709	252	81433	0.195	ng	99
38) Benzo(k)fluoranthene	22.753	252	82642	0.199	ng	97
39) Benzo(a)pyrene	23.277	252	72860	0.199	ng	99
40) Dibenzo(a,h)anthracene	25.618	278	76615	0.219	ng	99
41) Benzo(g,h,i)perylene	26.275	276	85746	0.220	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102921\
Data File : BN017182.D
Acq On : 29 Oct 2021 15:33
Operator : CG/JU
Sample : SSTDICC0.2
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2


Quant Time: Oct 29 17:24:01 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN102921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 29 17:22:00 2021
Response via : Initial Calibration








1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.560 min Scan# 497
 Delta R.T. -0.001 min
 Lab File: BN017182.D
 Acq: 29 Oct 2021 15:33

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.2







Tgt Ion:152 Resp: 31735
 Ion Ratio Lower Upper
 152 100
 150 154.3 124.6 187.0
 115 59.1 47.0 70.6



1,4-Dioxane
 Concen: 0.189 ng
 RT: 3.162 min Scan# 20
 Delta R.T. 0.009 min
 Lab File: BN017182.D
 Acq: 29 Oct 2021 15:33

Tgt Ion: 88 Resp: 3892
 Ion Ratio Lower Upper
 88 100
 43 292.7 103.8 155.6#
 58 91.6 70.6 106.0









n-Nitrosodimethylamine
Concen: 0.225 ng
RT: 3.494 min Scan# 56
Delta R.T. -0.000 min
Lab File: BN017182.D
Acq: 29 Oct 2021 15:33

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2

Tgt Ion: 42 Resp: 5537




Ion	Ratio	Lower	Upper
42	100		
74	125.8	100.5	150.7
44	6.9	5.2	7.8




2-Fluorophenol
Concen: 0.219 ng
RT: 5.172 min Scan# 238
Delta R.T. -0.000 min
Lab File: BN017182.D
Acq: 29 Oct 2021 15:33

Tgt Ion: 112 Resp: 14614

Ion	Ratio	Lower	Upper
112	100		
64	58.5	46.6	70.0
63	30.1	23.8	35.6









Phenol-d6
Concen: 0.202 ng
RT: 6.749 min Scan# 409
Delta R.T. -0.000 min
Lab File: BN017182.D
Acq: 29 Oct 2021 15:33




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2

Tgt Ion:	99	Resp:	15408
Ion	Ratio	Lower	Upper
99	100		
42	20.5	16.2	24.4
71	31.0	24.6	37.0




bis(2-Chloroethyl)ether
Concen: 0.205 ng
RT: 7.007 min Scan# 437
Delta R.T. -0.000 min
Lab File: BN017182.D
Acq: 29 Oct 2021 15:33

Tgt Ion:	93	Resp:	17991
Ion	Ratio	Lower	Upper
93	100		
63	80.5	64.5	96.7
95	33.0	26.6	39.8





Abundance Scan 738 (10.332 min): BN017183.D\data.ms (-737) (-)




Naphthalene-d8
Concen: 0.400 ng
RT: 10.332 min Scan# 738
Delta R.T. -0.000 min
Lab File: BN017182.D
Acq: 29 Oct 2021 15:33

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2


Tgt Ion:	136	Resp:	142939
Ion	Ratio	Lower	Upper
136	100		
137	11.0	8.8	13.2
54	6.5	4.8	7.2
68	4.8	3.6	5.4



Abundance Scan 738 (10.332 min): BN017182.D\data.ms (-722) (-)





Abundance Scan 610 (8.710 min): BN017183.D\data.ms (-606) (-)




Nitrobenzene-d5
Concen: 0.161 ng
RT: 8.709 min Scan# 610
Delta R.T. -0.000 min
Lab File: BN017182.D
Acq: 29 Oct 2021 15:33

Tgt Ion:	82	Resp:	14940
Ion	Ratio	Lower	Upper
82	100		
128	43.6	36.0	54.0
54	53.8	41.0	61.6




Abundance Scan 610 (8.709 min): BN017182.D\data.ms (-594) (-)





Abundance Scan 742 (10.383 min): BN017183.D\data.ms (-736) (-)

Naphthalene
Concen: 0.221 ng
RT: 10.382 min Scan# 742
Delta R.T. -0.000 min
Lab File: BN017182.D
Acq: 29 Oct 2021 15:33


Instrument :
BNA_N
ClientSampled :
SSTDIC0.2



Tgt Ion:	128	Resp:	82029
Ion	Ratio	Lower	Upper
128	100		
129	11.0	8.7	13.1
127	12.8	10.2	15.2





Abundance Scan 742 (10.382 min): BN017182.D\data.ms (-734) (-)




Abundance Scan 765 (10.674 min): BN017183.D\data.ms (-760) (-)


Hexachlorobutadiene
Concen: 0.201 ng
RT: 10.674 min Scan# 765
Delta R.T. -0.000 min
Lab File: BN017182.D
Acq: 29 Oct 2021 15:33

Tgt Ion:	225	Resp:	14791
Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	63.5	51.0	76.4




Abundance Scan 765 (10.674 min): BN017182.D\data.ms (-757) (-)








Scan 925 (11.929 min): BN017183.D\data.ms (-912) (#11)
 2-Methylnaphthalene-d10
 Concen: 0.207 ng
 RT: 11.928 min Scan# 925
 Delta R.T. -0.000 min
 Lab File: BN017182.D
 Acq: 29 Oct 2021 15:33

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.2






Tgt Ion:152 Resp: 42048
 Ion Ratio Lower Upper
 152 100
 151 20.6 15.9 23.9



Scan 941 (12.000 min): BN017183.D\data.ms (-936) (#12)
 2-Methylnaphthalene
 Concen: 0.211 ng
 RT: 12.004 min Scan# 942
 Delta R.T. 0.004 min
 Lab File: BN017182.D
 Acq: 29 Oct 2021 15:33


Tgt Ion:142 Resp: 50496
 Ion Ratio Lower Upper
 142 100
 141 87.6 71.0 106.6
 115 32.4 26.8 40.2






Abundance Scan 1188 (14.194 min): BN017183.D\data.ms (-1119) (-)

Acenaphthene-d10
Concen: 0.400 ng
RT: 14.194 min Scan# 1188
Delta R.T. -0.000 min
Lab File: BN017182.D
Acq: 29 Oct 2021 15:33

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2







Tgt Ion:	164	Resp:	73172
Ion	Ratio	Lower	Upper
164	100		
162	104.8	83.6	125.4
160	48.5	38.3	57.5




Abundance Scan 1307 (15.704 min): BN017183.D\data.ms (-1204) (-)

2,4,6-Tribromophenol
Concen: 0.136 ng
RT: 15.704 min Scan# 1307
Delta R.T. -0.000 min
Lab File: BN017182.D
Acq: 29 Oct 2021 15:33

Tgt Ion:	330	Resp:	4042
Ion	Ratio	Lower	Upper
330	100		
332	0.0	0.0	0.0
141	39.0	30.7	46.1









2-Fluorobiphenyl
 Concen: 0.216 ng
 RT: 12.823 min Scan# 1080
 Delta R.T. -0.000 min
 Lab File: BN017182.D
 Acq: 29 Oct 2021 15:33




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.2

Tgt Ion:	172	Resp:	59195
Ion	Ratio	Lower	Upper
172	100		
171	34.1	27.0	40.6
170	22.1	17.5	26.3



Acenaphthylene
 Concen: 0.185 ng
 RT: 13.915 min Scan# 1166
 Delta R.T. -0.000 min
 Lab File: BN017182.D
 Acq: 29 Oct 2021 15:33


Tgt Ion:	152	Resp:	54747
Ion	Ratio	Lower	Upper
152	100		
151	19.4	15.6	23.4
153	13.0	10.4	15.6






Abundance Scan 1193 (14.257 min): BN017183.D\data.ms (-1187) (-)

Acenaphthene
Concen: 0.212 ng
RT: 14.257 min Scan# 1193
Delta R.T. -0.000 min
Lab File: BN017182.D
Acq: 29 Oct 2021 15:33

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2




Tgt Ion	Ratio	Lower	Upper
154	100		
153	114.2	91.1	136.7
152	55.5	44.4	66.6







Abundance Scan 1272 (15.259 min): BN017183.D\data.ms (-1266) (-)

Fluorene
Concen: 0.203 ng
RT: 15.259 min Scan# 1272
Delta R.T. -0.000 min
Lab File: BN017182.D
Acq: 29 Oct 2021 15:33



Tgt Ion	Ratio	Lower	Upper
166	100		
165	97.3	78.4	117.6
167	13.5	10.8	16.2









Scan 1408 (16.946 min): BN017183.D\data.ms (-1399) (-)
 Phenanthrene-d10
 Concen: 0.400 ng
 RT: 16.946 min Scan# 1408
 Delta R.T. -0.000 min
 Lab File: BN017182.D
 Acq: 29 Oct 2021 15:33




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.2

Tgt Ion:	188	Resp:	133238
Ion Ratio	Lower	Upper	
188	100		
94	0.0	0.0	0.0
80	12.1	10.3	15.5




Scan 1279 (15.349 min): BN017183.D\data.ms (-1729) (-)
 4,6-Dinitro-2-methylphenol
 Concen: 0.135 ng
 RT: 15.348 min Scan# 1279
 Delta R.T. -0.000 min
 Lab File: BN017182.D
 Acq: 29 Oct 2021 15:33

Tgt Ion:	198	Resp:	1899
Ion Ratio	Lower	Upper	
198	100		
182	17.9	11.4	17.2#
77	0.0	0.0	0.0






Abundance Scan 1343 (16.155 min): BN017183.D\data.ms (-1335) (-)




4-Bromophenyl-phenylether
Concen: 0.188 ng
RT: 16.155 min Scan# 1343
Delta R.T. -0.000 min
Lab File: BN017182.D
Acq: 29 Oct 2021 15:33

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2

Tgt Ion:	248	Resp:	14621
Ion	Ratio	Lower	Upper
248	100		
250	96.6	77.4	116.0
141	55.7	44.2	66.4






Abundance Scan 1352 (16.264 min): BN017183.D\data.ms (-1344) (-)



Hexachlorobenzene
Concen: 0.190 ng
RT: 16.264 min Scan# 1352
Delta R.T. -0.000 min
Lab File: BN017182.D
Acq: 29 Oct 2021 15:33


Tgt Ion:	284	Resp:	16927
Ion	Ratio	Lower	Upper
284	100		
142	36.7	29.0	43.4
249	30.8	24.5	36.7





Abundance Scan 1366 (16.435 min): BN017183.D\data.ms (-1323) (-)

Atrazine
Concen: 0.166 ng
RT: 16.434 min Scan# 1366
Delta R.T. -0.000 min
Lab File: BN017182.D
Acq: 29 Oct 2021 15:33


Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2



Tgt Ion:	200	Resp:	8553
Ion Ratio	Lower	Upper	
200	100		
173	27.2	21.7	32.5
215	48.2	37.8	56.6




Abundance Scan 1366 (16.434 min): BN017182.D\data.ms (-1325) (-)





Abundance Scan 1380 (16.605 min): BN017183.D\data.ms (-1324) (-)


Pentachlorophenol
Concen: 0.154 ng
RT: 16.617 min Scan# 1381
Delta R.T. 0.012 min
Lab File: BN017182.D
Acq: 29 Oct 2021 15:33



Tgt Ion:	266	Resp:	3782
Ion Ratio	Lower	Upper	
266	100		
264	62.9	50.3	75.5
268	62.6	50.7	76.1




Abundance Scan 1381 (16.617 min): BN017182.D\data.ms (-1372) (-)






Abundance Scan 1412 (16.995 min): BN017183.D\data.ms (-1425) (-)

Phenanthrene
Concen: 0.209 ng
RT: 16.994 min Scan# 1412
Delta R.T. -0.000 min
Lab File: BN017182.D
Acq: 29 Oct 2021 15:33

Instrument :
BNA_N
ClientSampled :
SSTDIC0.2







Tgt Ion:	178	Resp:	79104
Ion	Ratio	Lower	Upper
178	100		
176	18.8	15.0	22.4
179	15.5	12.3	18.5



Abundance Scan 1419 (17.080 min): BN017183.D\data.ms (-1426) (-)

Anthracene
Concen: 0.182 ng
RT: 17.079 min Scan# 1419
Delta R.T. -0.000 min
Lab File: BN017182.D
Acq: 29 Oct 2021 15:33


Tgt Ion:	178	Resp:	58310
Ion	Ratio	Lower	Upper
178	100		
176	18.1	14.8	22.2
179	15.3	12.2	18.4





Abundance Scan 1693 (18.995 min): BN017183.D\data.ms (-1627) (-)

Fluoranthene-d10
Concen: 0.196 ng
RT: 18.994 min Scan# 1693
Delta R.T. -0.000 min
Lab File: BN017182.D
Acq: 29 Oct 2021 15:33


Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2



Tgt Ion:	212	Resp:	65519
Ion Ratio	Lower	Upper	
212	100		
106	13.0	10.6	15.8
104	7.2	5.8	8.6




Abundance Scan 1693 (18.994 min): BN017182.D\data.ms (-1673) (-)





Abundance Scan 1699 (19.025 min): BN017183.D\data.ms (-1628) (-)

Fluoranthene
Concen: 0.200 ng
RT: 19.024 min Scan# 1699
Delta R.T. -0.000 min
Lab File: BN017182.D
Acq: 29 Oct 2021 15:33


Tgt Ion:	202	Resp:	82290
Ion Ratio	Lower	Upper	
202	100		
101	11.1	9.0	13.4
203	17.2	13.8	20.8



Abundance Scan 1699 (19.024 min): BN017182.D\data.ms (-1659) (-)






Abundance Scan 2006 (21.165 min): BN017183.D\data.ms (-1987) (-)




Chrysene-d12
Concen: 0.400 ng
RT: 21.165 min Scan# 2006
Delta R.T. -0.000 min
Lab File: BN017182.D
Acq: 29 Oct 2021 15:33

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2

Tgt Ion:	240	Resp:	122711
Ion	Ratio	Lower	Upper
240	100		
120	6.3	5.0	7.4
236	25.5	20.3	30.5






Abundance Scan 1773 (19.392 min): BN017183.D\data.ms (-1733) (-)



Pyrene
Concen: 0.210 ng
RT: 19.392 min Scan# 1773
Delta R.T. -0.000 min
Lab File: BN017182.D
Acq: 29 Oct 2021 15:33


Tgt Ion:	202	Resp:	81190
Ion	Ratio	Lower	Upper
202	100		
200	20.6	16.5	24.7
203	17.4	14.0	21.0






Abundance Scan 1817 (19.610 min): BN017183.D\data.ms (-1834) (-)

Terphenyl-d14
Concen: 0.203 ng
RT: 19.610 min Scan# 1817
Delta R.T. -0.000 min
Lab File: BN017182.D
Acq: 29 Oct 2021 15:33

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2

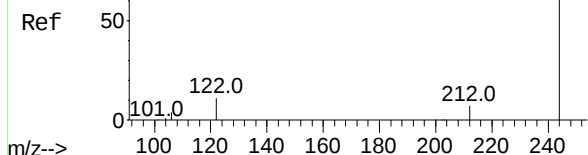


Tgt Ion	Ratio	Lower	Upper
244	100		
212	7.4	5.8	8.6
122	11.7	9.2	13.8







Abundance Scan 2004 (21.144 min): BN017183.D\data.ms (-1932) (-)

Benzo(a)anthracene
Concen: 0.193 ng
RT: 21.144 min Scan# 2004
Delta R.T. -0.000 min
Lab File: BN017182.D
Acq: 29 Oct 2021 15:33



Tgt Ion	Ratio	Lower	Upper
228	100		
226	27.2	21.9	32.9
229	19.3	15.4	23.2









Chrysene
 Concen: 0.212 ng
 RT: 21.197 min Scan# 2009
 Delta R.T. -0.000 min
 Lab File: BN017182.D
 Acq: 29 Oct 2021 15:33




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.2

Tgt Ion	Ratio	Lower	Upper
228	100		
226	29.5	23.6	35.4
229	19.4	15.5	23.3



Bis(2-ethylhexyl)phthalate
 Concen: 0.155 ng
 RT: 21.101 min Scan# 2000
 Delta R.T. -0.000 min
 Lab File: BN017182.D
 Acq: 29 Oct 2021 15:33


Tgt Ion	Ratio	Lower	Upper
149	100		
167	27.1	21.6	32.4
279	4.2	3.2	4.8






Abundance Scan 2406 (23.376 min): BN017183.D\data.ms (-305) (-)

Perylene-d12
Concen: 0.400 ng
RT: 23.373 min Scan# 2405
Delta R.T. -0.004 min
Lab File: BN017182.D
Acq: 29 Oct 2021 15:33

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2







Tgt Ion	Ratio	Lower	Upper
264	100		
260	24.6	19.4	29.0
265	23.1	18.2	27.4




Abundance Scan 3055 (25.597 min): BN017183.D\data.ms (-3036) (-)

Indeno(1,2,3-cd)pyrene
Concen: 0.221 ng
RT: 25.597 min Scan# 3055
Delta R.T. -0.000 min
Lab File: BN017182.D
Acq: 29 Oct 2021 15:33

Tgt Ion	Ratio	Lower	Upper
276	100		
138	25.9	20.4	30.6
277	25.0	20.0	30.0






Abundance Scan 2212 (22.712 min): BN017183.D\data.ms (-2154) (-)




Benzo(b)fluoranthene
Concen: 0.195 ng
RT: 22.709 min Scan# 2211
Delta R.T. -0.004 min
Lab File: BN017182.D
Acq: 29 Oct 2021 15:33

Tgt Ion:	252	Resp:	81433
Ion	Ratio	Lower	Upper
252	100		
253	22.2	17.5	26.3
125	10.5	7.9	11.9






Abundance Scan 2224 (22.753 min): BN017183.D\data.ms (-2209) (-)



Benzo(k)fluoranthene
Concen: 0.199 ng
RT: 22.753 min Scan# 2224
Delta R.T. -0.000 min
Lab File: BN017182.D
Acq: 29 Oct 2021 15:33

Tgt Ion:	252	Resp:	82642
Ion	Ratio	Lower	Upper
252	100		
253	22.8	17.6	26.4
125	13.1	9.2	13.8




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2




Abundance Scan 2376 (23.274 min): BN017183.D\data.ms (-339) (-)

Benzo(a)pyrene
Concen: 0.199 ng
RT: 23.277 min Scan# 2377
Delta R.T. 0.003 min
Lab File: BN017182.D
Acq: 29 Oct 2021 15:33

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2




Tgt Ion:	252	Resp:	72860
Ion Ratio	Lower	Upper	
252	100		
253	22.8	17.6	26.4
125	11.6	9.1	13.7






Abundance Scan 3062 (25.622 min): BN017183.D\data.ms (-3033) (-)


Dibenzo(a,h)anthracene
Concen: 0.219 ng
RT: 25.618 min Scan# 3061
Delta R.T. -0.004 min
Lab File: BN017182.D
Acq: 29 Oct 2021 15:33



Tgt Ion:	278	Resp:	76615
Ion Ratio	Lower	Upper	
278	100		
139	17.3	13.2	19.8
279	24.0	19.0	28.6




Abundance Scan 3253 (26.275 min): BN017183.D\data.ms (-3223) (-)




Benzo(g,h,i)perylene
Concen: 0.220 ng
RT: 26.275 min Scan# 3253
Delta R.T. -0.000 min
Lab File: BN017182.D
Acq: 29 Oct 2021 15:33

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2

Abundance Scan 3253 (26.275 min): BN017182.D\data.ms



Tgt Ion:	276	Resp:	85746
Ion	Ratio	Lower	Upper
276	100		
277	23.8	19.0	28.4
138	21.6	17.4	26.0



Abundance Scan 3253 (26.275 min): BN017182.D\data.ms (-3195) (-)

