

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102921\
 Data File : BN017183.D
 Acq On : 29 Oct 2021 16:51
 Operator : CG/JU
 Sample : SSTDICCC0.4
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICCC0.4

Quant Time: Oct 29 17:23:03 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN102921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 29 17:22:00 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.561	152	33338	0.400	ng	0.00
7) Naphthalene-d8	10.332	136	148881	0.400	ng	0.00
13) Acenaphthene-d10	14.194	164	77264	0.400	ng	0.00
19) Phenanthrene-d10	16.946	188	140825	0.400	ng	0.00
29) Chrysene-d12	21.165	240	138952	0.400	ng	0.00
35) Perylene-d12	23.376	264	137350	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.173	112	26011	0.372	ng	0.00
5) Phenol-d6	6.749	99	28698	0.358	ng	0.00
8) Nitrobenzene-d5	8.710	82	28156	0.292	ng	0.00
11) 2-Methylnaphthalene-d10	11.929	152	127753	0.605	ng	0.00
14) 2,4,6-Tribromophenol	15.704	330	8412	0.268	ng	0.00
15) 2-Fluorobiphenyl	12.824	172	110275	0.381	ng	0.00
27) Fluoranthene-d10	18.995	212	221203	0.628	ng	0.00
31) Terphenyl-d14	19.610	244	112322	0.365	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.153	88	6459	0.298	ng	99
3) n-Nitrosodimethylamine	3.494	42	10301	0.399	ng	99
6) bis(2-Chloroethyl)ether	7.008	93	32551	0.353	ng	100
9) Naphthalene	10.383	128	145068	0.375	ng	100
10) Hexachlorobutadiene	10.674	225	26622	0.347	ng	# 100
12) 2-Methylnaphthalene	12.000	142	92743	0.372	ng	100
16) Acenaphthylene	13.915	152	109264	0.350	ng	100
17) Acenaphthene	14.257	154	80000	0.374	ng	100
18) Fluorene	15.260	166	94038	0.365	ng	100
20) 4,6-Dinitro-2-methylph...	15.349	198	3823	0.258	ng	100
21) 4-Bromophenyl-phenylether	16.155	248	28587	0.348	ng	100
22) Hexachlorobenzene	16.264	284	32150	0.341	ng	100
23) Atrazine	16.435	200	17524	0.322	ng	100
24) Pentachlorophenol	16.605	266	8007	0.308	ng	100
25) Phenanthrene	16.995	178	151880	0.379	ng	100
26) Anthracene	17.080	178	118099	0.349	ng	100
28) Fluoranthene	19.025	202	167170	0.384	ng	100
30) Pyrene	19.392	202	163050	0.372	ng	100
32) Benzo(a)anthracene	21.144	228	147813	0.360	ng	100
33) Chrysene	21.197	228	165808	0.367	ng	100
34) Bis(2-ethylhexyl)phtha...	21.101	149	48088	0.271	ng	100
36) Indeno(1,2,3-cd)pyrene	25.598	276	186931	0.399	ng	100
37) Benzo(b)fluoranthene	22.712	252	161395	0.360	ng	100
38) Benzo(k)fluoranthene	22.753	252	162581	0.365	ng	100
39) Benzo(a)pyrene	23.274	252	141811	0.362	ng	100
40) Dibenzo(a,h)anthracene	25.622	278	151026	0.403	ng	100
41) Benzo(g,h,i)perylene	26.275	276	164255	0.393	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102921\
Data File : BN017183.D
Acq On : 29 Oct 2021 16:51
Operator : CG/JU
Sample : SSTDICCC0.4
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

Quant Time: Oct 29 17:23:03 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN102921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 29 17:22:00 2021
Response via : Initial Calibration

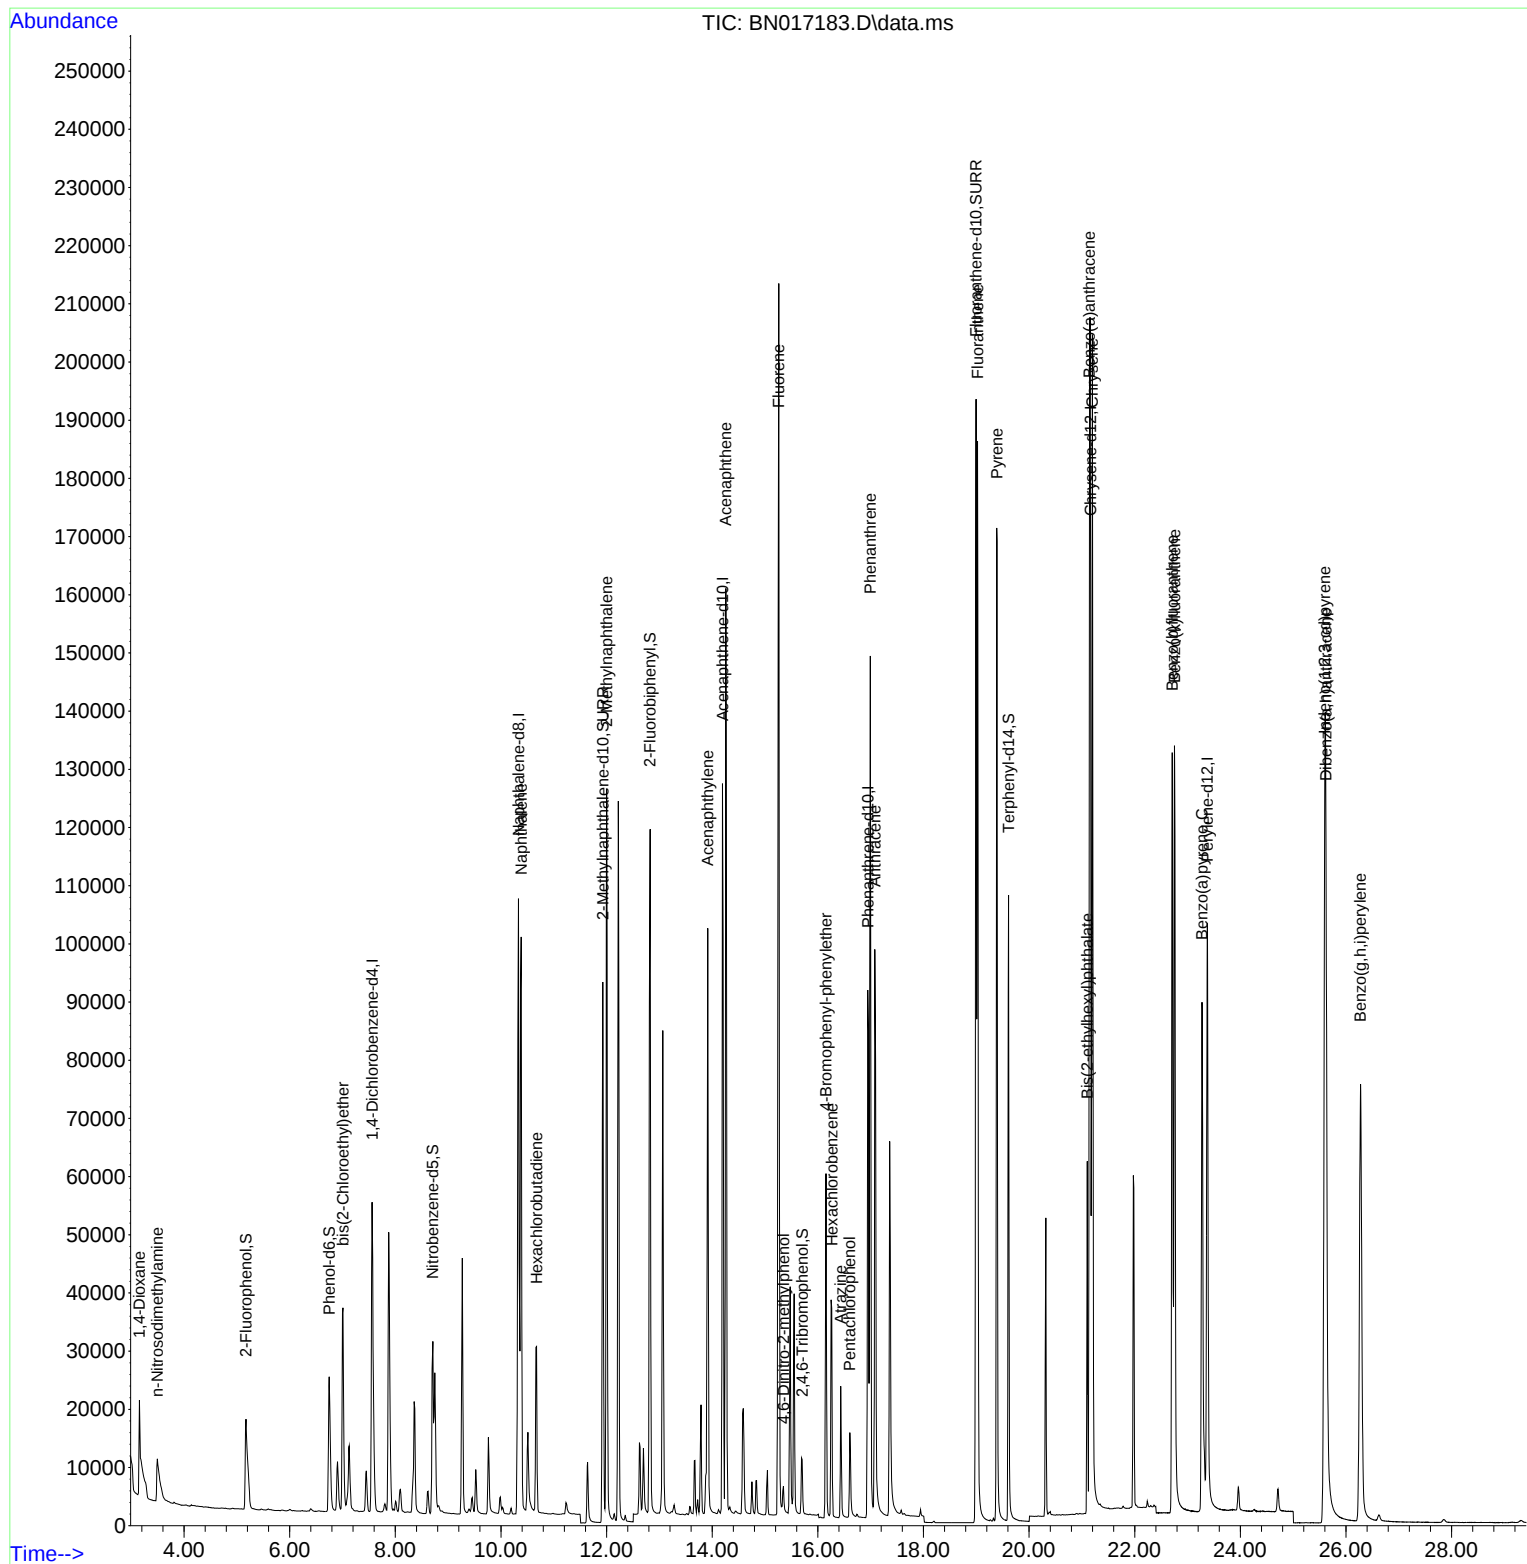







#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.561 min Scan# 497
 Delta R.T. -0.000 min
 Lab File: BN017183.D
 Acq: 29 Oct 2021 16:51

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.4

Tgt Ion:152 Resp: 33338




Ion	Ratio	Lower	Upper
152	100		
150	155.8	124.6	187.0
115	58.8	47.0	70.6

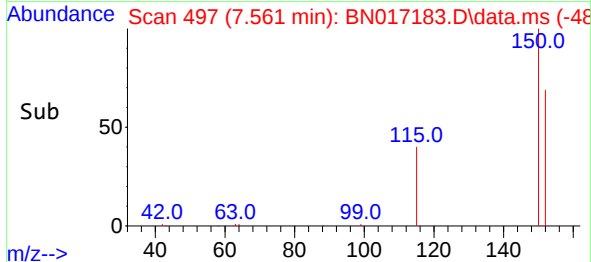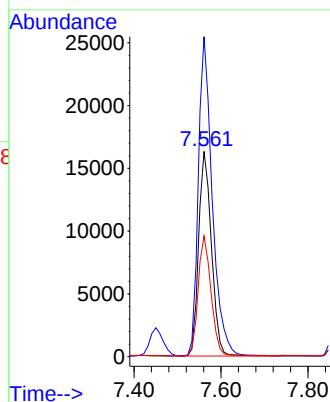




#2
 1,4-Dioxane
 Concen: 0.298 ng
 RT: 3.153 min Scan# 19
 Delta R.T. 0.000 min
 Lab File: BN017183.D
 Acq: 29 Oct 2021 16:51

Tgt Ion: 88 Resp: 6459

Ion	Ratio	Lower	Upper
88	100		
43	128.6	103.8	155.6
58	87.0	70.6	106.0

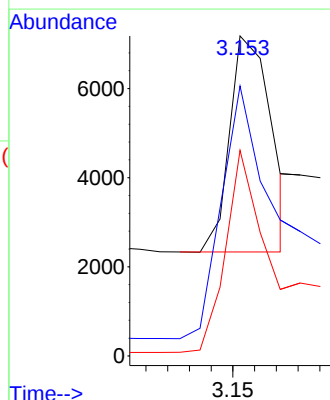





Abundance Scan 56 (3.494 min): BN017183.D\data.ms (-52)

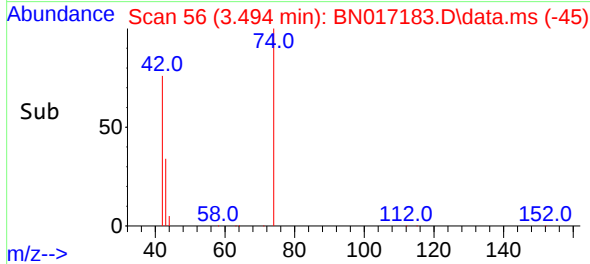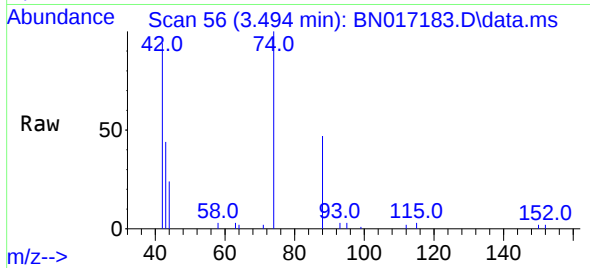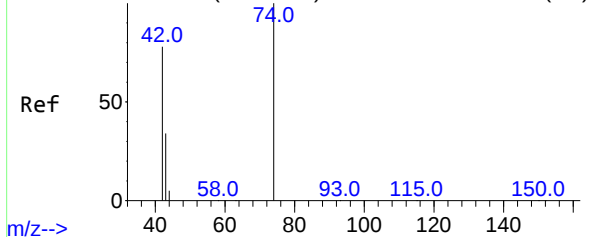

#3

n-Nitrosodimethylamine
Concen: 0.399 ng
RT: 3.494 min Scan# 56
Delta R.T. 0.000 min
Lab File: BN017183.D
Acq: 29 Oct 2021 16:51


Tgt Ion:	42	Resp:	10301
Ion	Ratio	Lower	Upper
42	100		
74	124.6	100.5	150.7
44	6.8	5.2	7.8

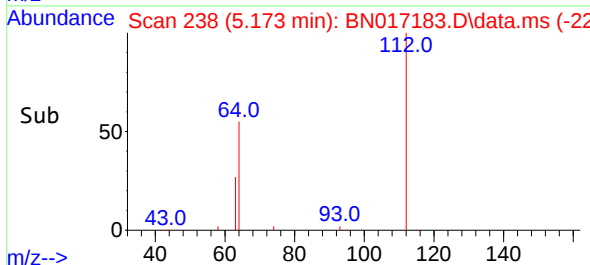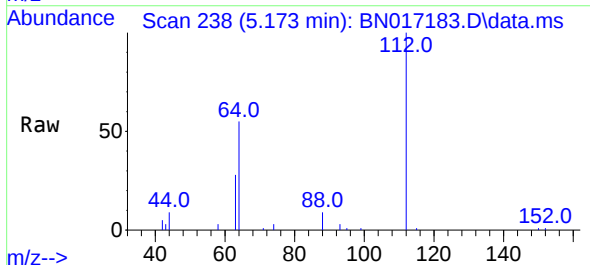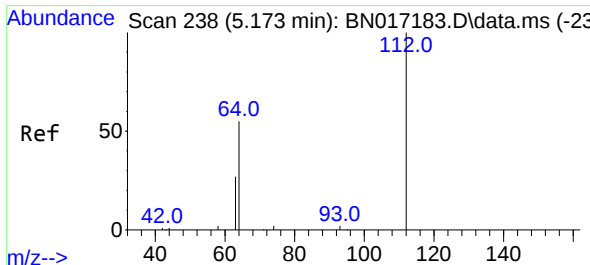


#4

2-Fluorophenol
Concen: 0.372 ng
RT: 5.173 min Scan# 238
Delta R.T. 0.000 min
Lab File: BN017183.D
Acq: 29 Oct 2021 16:51

Tgt Ion:	112	Resp:	26011
Ion	Ratio	Lower	Upper
112	100		
64	58.4	46.6	70.0
63	29.7	23.8	35.6

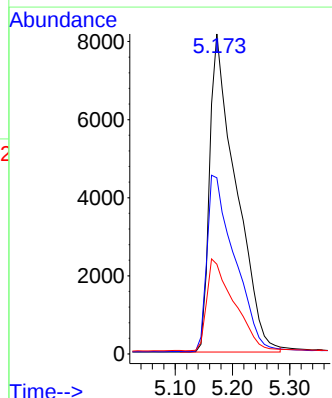

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4







#5
Phenol-d6
Concen: 0.358 ng
RT: 6.749 min Scan# 409
Delta R.T. 0.000 min
Lab File: BN017183.D
Acq: 29 Oct 2021 16:51

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

Tgt Ion: 99 Resp: 28698




Ion	Ratio	Lower	Upper
99	100		
42	20.3	16.2	24.4
71	30.8	24.6	37.0




#6
bis(2-Chloroethyl)ether
Concen: 0.353 ng
RT: 7.008 min Scan# 437
Delta R.T. 0.000 min
Lab File: BN017183.D
Acq: 29 Oct 2021 16:51

Tgt Ion: 93 Resp: 32551

Ion	Ratio	Lower	Upper
93	100		
63	80.6	64.5	96.7
95	33.2	26.6	39.8

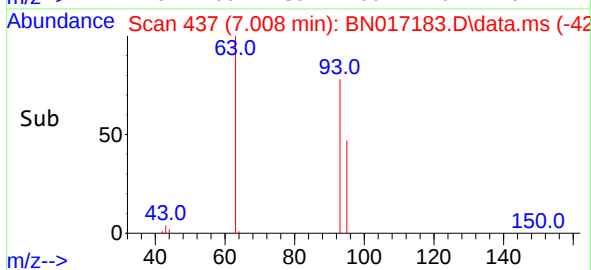







#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.332 min Scan# 738
Delta R.T. 0.000 min
Lab File: BN017183.D
Acq: 29 Oct 2021 16:51

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

Tgt Ion: 136 Resp: 148881




Ion	Ratio	Lower	Upper
136	100		
137	11.0	8.8	13.2
54	6.0	4.8	7.2
68	4.5	3.6	5.4

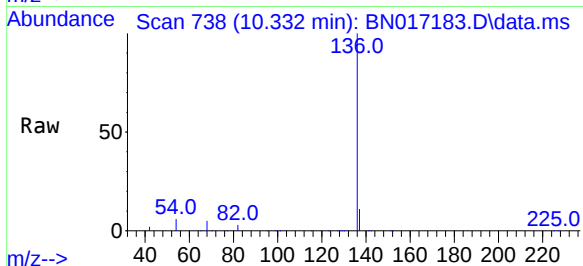


#8
Nitrobenzene-d5
Concen: 0.292 ng
RT: 8.710 min Scan# 610
Delta R.T. 0.000 min
Lab File: BN017183.D
Acq: 29 Oct 2021 16:51

Tgt Ion: 82 Resp: 28156

Ion	Ratio	Lower	Upper
82	100		
128	45.0	36.0	54.0
54	51.3	41.0	61.6



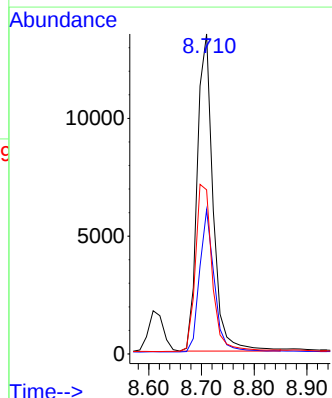
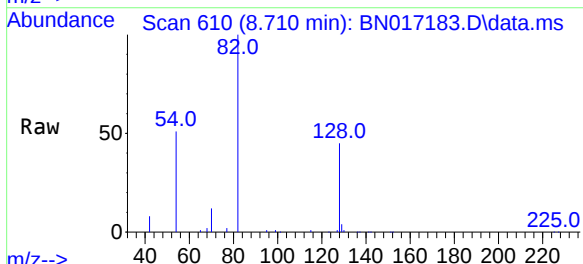




#9
Naphthalene
Concen: 0.375 ng
RT: 10.383 min Scan# 742
Delta R.T. 0.000 min
Lab File: BN017183.D
Acq: 29 Oct 2021 16:51




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:128 Resp: 145068
Ion Ratio Lower Upper
128 100
129 10.9 8.7 13.1
127 12.7 10.2 15.2



#10
Hexachlorobutadiene
Concen: 0.347 ng
RT: 10.674 min Scan# 765
Delta R.T. 0.000 min
Lab File: BN017183.D
Acq: 29 Oct 2021 16:51

Tgt Ion:225 Resp: 26622
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 63.7 51.0 76.4


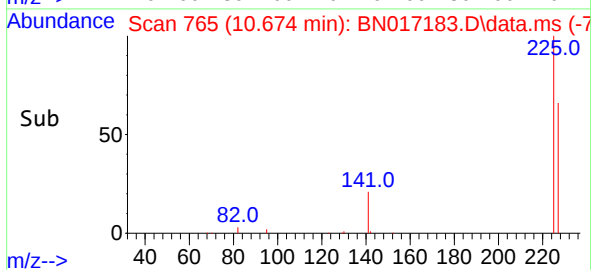




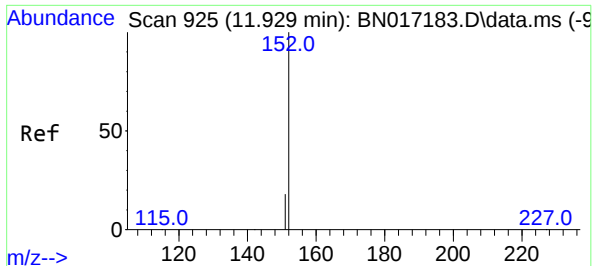

#11
2-Methylnaphthalene-d10
Concen: 0.605 ng
RT: 11.929 min Scan# 925
Delta R.T. 0.000 min
Lab File: BN017183.D
Acq: 29 Oct 2021 16:51




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:152 Resp: 127753
Ion Ratio Lower Upper
152 100
151 19.9 15.9 23.9

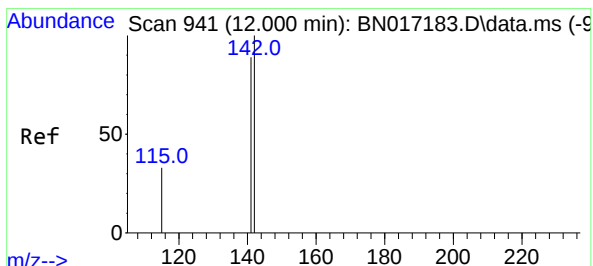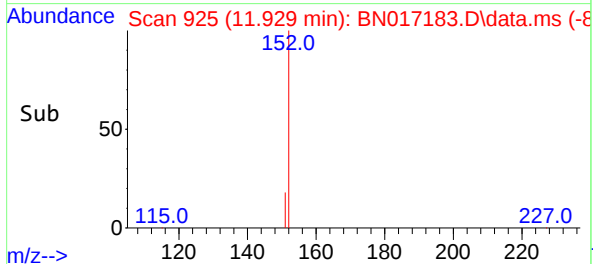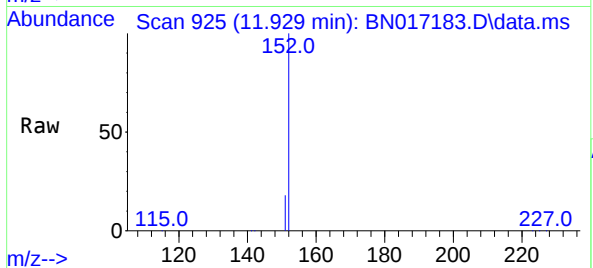

#12
2-Methylnaphthalene
Concen: 0.372 ng
RT: 12.000 min Scan# 941
Delta R.T. 0.000 min
Lab File: BN017183.D
Acq: 29 Oct 2021 16:51

Tgt Ion:142 Resp: 92743
Ion Ratio Lower Upper
142 100
141 88.8 71.0 106.6
115 33.5 26.8 40.2


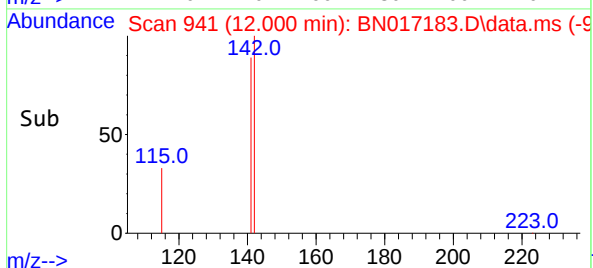

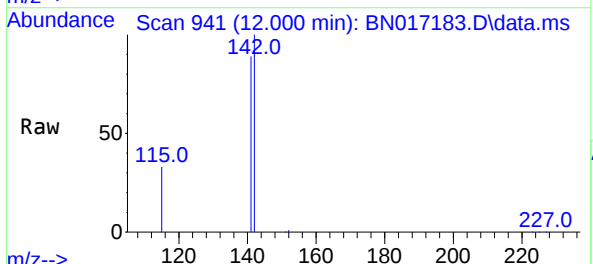




#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.194 min Scan# 1188
Delta R.T. 0.000 min
Lab File: BN017183.D
Acq: 29 Oct 2021 16:51




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:164 Resp: 77264
Ion Ratio Lower Upper
164 100
162 104.5 83.6 125.4
160 47.9 38.3 57.5

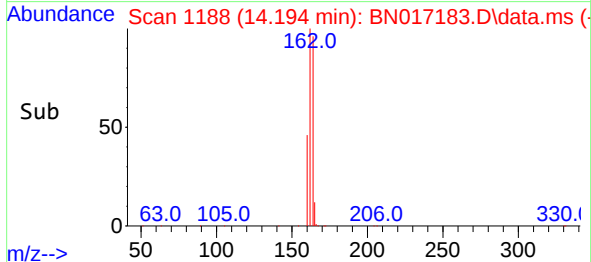

#14
2,4,6-Tribromophenol
Concen: 0.268 ng
RT: 15.704 min Scan# 1307
Delta R.T. 0.000 min
Lab File: BN017183.D
Acq: 29 Oct 2021 16:51

Tgt Ion:330 Resp: 8412
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 38.3 30.7 46.1


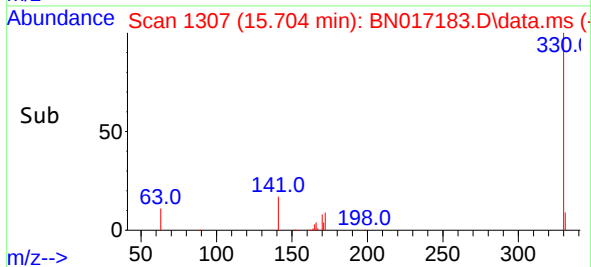

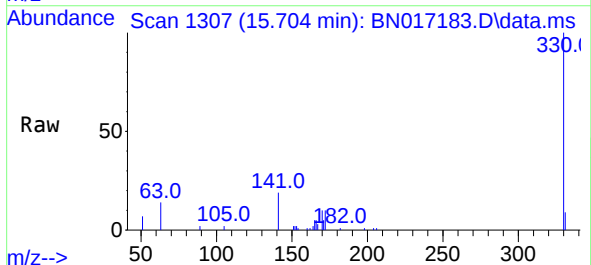


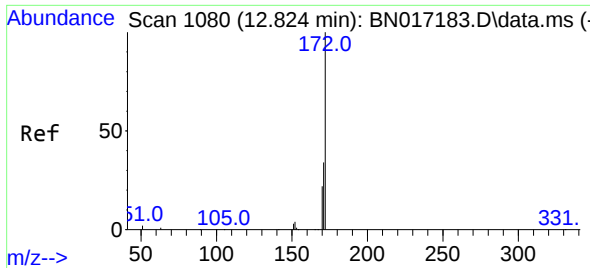

#15
2-Fluorobiphenyl
Concen: 0.381 ng
RT: 12.824 min Scan# 1080
Delta R.T. 0.000 min
Lab File: BN017183.D
Acq: 29 Oct 2021 16:51




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:172 Resp: 110275
Ion Ratio Lower Upper
172 100
171 33.8 27.0 40.6
170 21.9 17.5 26.3

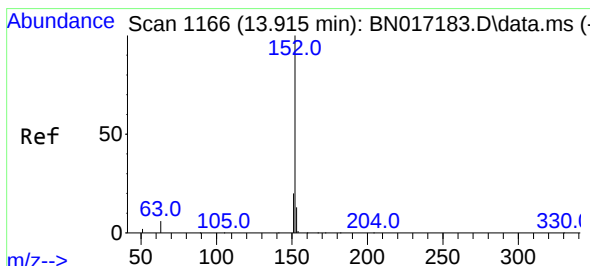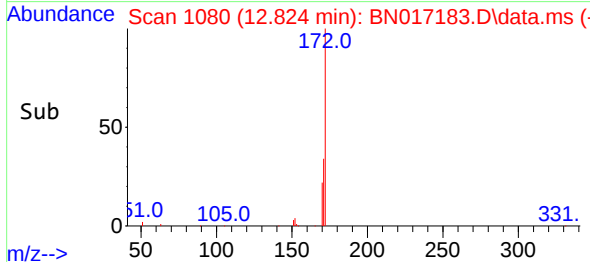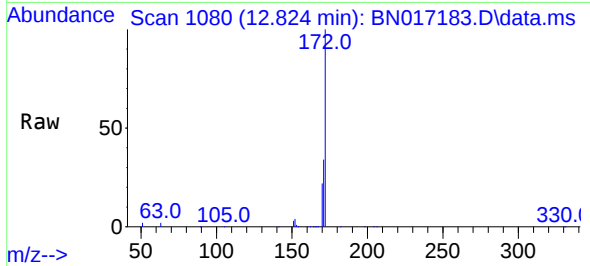

#16
Acenaphthylene
Concen: 0.350 ng
RT: 13.915 min Scan# 1166
Delta R.T. 0.000 min
Lab File: BN017183.D
Acq: 29 Oct 2021 16:51

Tgt Ion:152 Resp: 109264
Ion Ratio Lower Upper
152 100
151 19.5 15.6 23.4
153 13.0 10.4 15.6


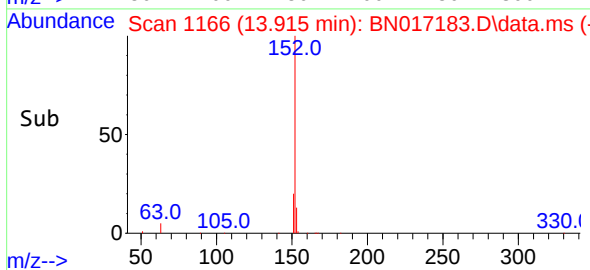

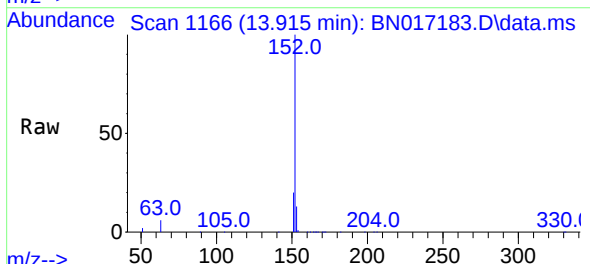




#17
Acenaphthene
Concen: 0.374 ng
RT: 14.257 min Scan# 1193
Delta R.T. 0.000 min
Lab File: BN017183.D
Acq: 29 Oct 2021 16:51




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:154 Resp: 80000
Ion Ratio Lower Upper
154 100
153 113.9 91.1 136.7
152 55.5 44.4 66.6



#18
Fluorene
Concen: 0.365 ng
RT: 15.260 min Scan# 1272
Delta R.T. 0.000 min
Lab File: BN017183.D
Acq: 29 Oct 2021 16:51

Tgt Ion:166 Resp: 94038
Ion Ratio Lower Upper
166 100
165 98.0 78.4 117.6
167 13.5 10.8 16.2


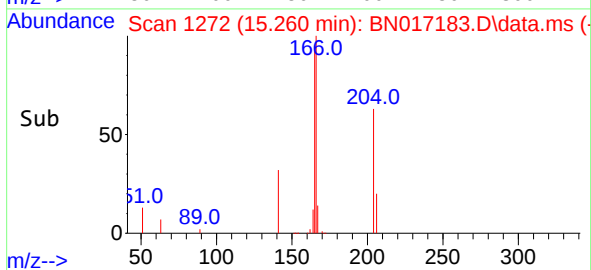

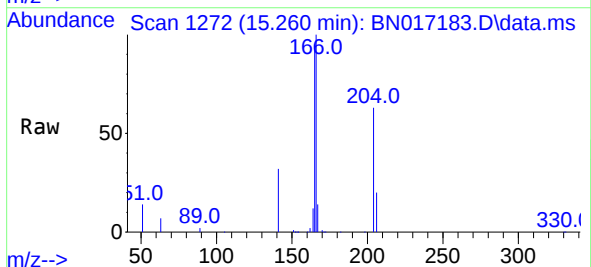




#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 16.946 min Scan# 1408
Delta R.T. 0.000 min
Lab File: BN017183.D
Acq: 29 Oct 2021 16:51




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:188 Resp: 140825
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 12.9 10.3 15.5



#20
4,6-Dinitro-2-methylphenol
Concen: 0.258 ng
RT: 15.349 min Scan# 1279
Delta R.T. 0.000 min
Lab File: BN017183.D
Acq: 29 Oct 2021 16:51

Tgt Ion:198 Resp: 3823
Ion Ratio Lower Upper
198 100
182 14.3 11.4 17.2
77 0.0 0.0 0.0


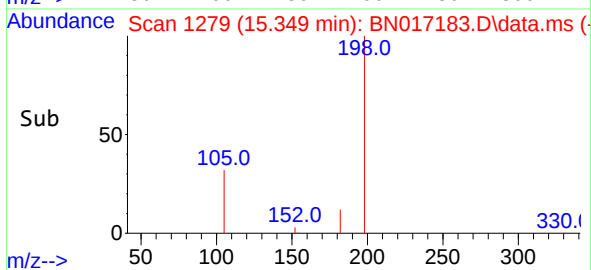






#21
4-Bromophenyl-phenylether
Concen: 0.348 ng
RT: 16.155 min Scan# 1343
Delta R.T. 0.000 min
Lab File: BN017183.D
Acq: 29 Oct 2021 16:51




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:	248	Resp:	28587
Ion	Ratio	Lower	Upper
248	100		
250	96.7	77.4	116.0
141	55.3	44.2	66.4

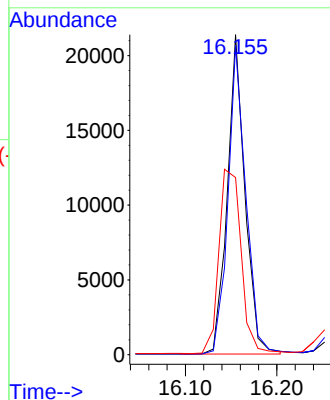

#22
Hexachlorobenzene
Concen: 0.341 ng
RT: 16.264 min Scan# 1352
Delta R.T. 0.000 min
Lab File: BN017183.D
Acq: 29 Oct 2021 16:51

Tgt Ion:	284	Resp:	32150
Ion	Ratio	Lower	Upper
284	100		
142	36.2	29.0	43.4
249	30.6	24.5	36.7


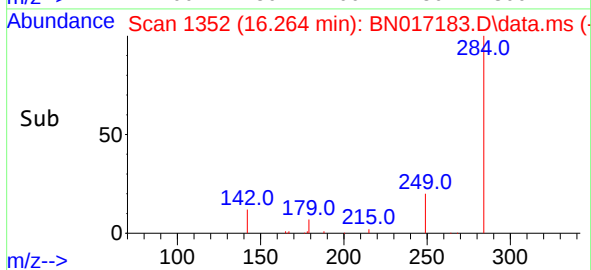
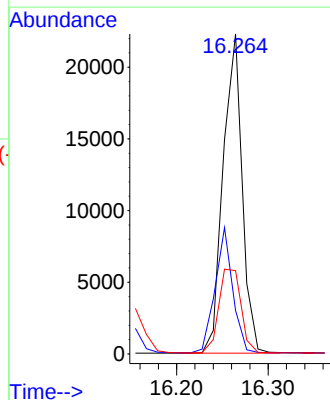





#23
Atrazine
Concen: 0.322 ng
RT: 16.435 min Scan# 1366
Delta R.T. 0.000 min
Lab File: BN017183.D
Acq: 29 Oct 2021 16:51




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:200 Resp: 17524
Ion Ratio Lower Upper
200 100
173 27.1 21.7 32.5
215 47.2 37.8 56.6

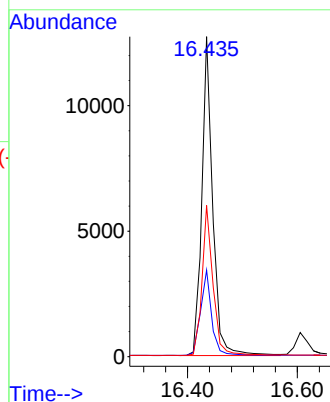

#24
Pentachlorophenol
Concen: 0.308 ng
RT: 16.605 min Scan# 1380
Delta R.T. 0.000 min
Lab File: BN017183.D
Acq: 29 Oct 2021 16:51

Tgt Ion:266 Resp: 8007
Ion Ratio Lower Upper
266 100
264 62.9 50.3 75.5
268 63.4 50.7 76.1



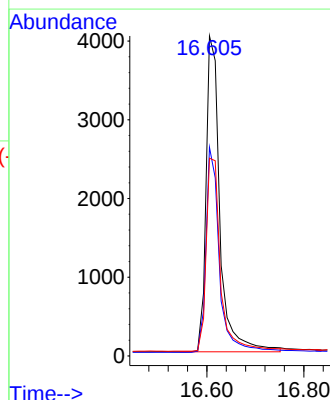





#25
Phenanthrene
Concen: 0.379 ng
RT: 16.995 min Scan# 1412
Delta R.T. 0.000 min
Lab File: BN017183.D
Acq: 29 Oct 2021 16:51




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:178 Resp: 151880
Ion Ratio Lower Upper
178 100
176 18.7 15.0 22.4
179 15.4 12.3 18.5



#26
Anthracene
Concen: 0.349 ng
RT: 17.080 min Scan# 1419
Delta R.T. 0.000 min
Lab File: BN017183.D
Acq: 29 Oct 2021 16:51

Tgt Ion:178 Resp: 118099
Ion Ratio Lower Upper
178 100
176 18.5 14.8 22.2
179 15.3 12.2 18.4


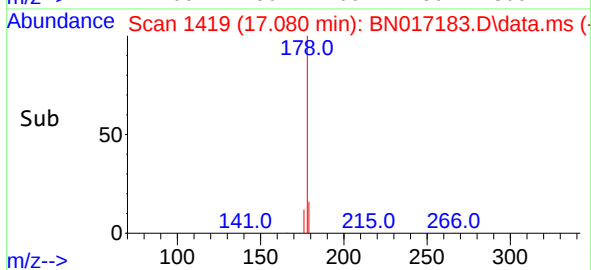






#27
Fluoranthene-d10
Concen: 0.628 ng
RT: 18.995 min Scan# 1693
Delta R.T. 0.000 min
Lab File: BN017183.D
Acq: 29 Oct 2021 16:51




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:212 Resp: 221203
Ion Ratio Lower Upper
212 100
106 13.2 10.6 15.8
104 7.2 5.8 8.6

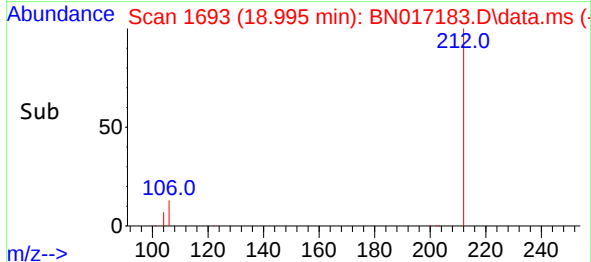

#28
Fluoranthene
Concen: 0.384 ng
RT: 19.025 min Scan# 1699
Delta R.T. 0.000 min
Lab File: BN017183.D
Acq: 29 Oct 2021 16:51

Tgt Ion:202 Resp: 167170
Ion Ratio Lower Upper
202 100
101 11.2 9.0 13.4
203 17.4 13.8 20.8

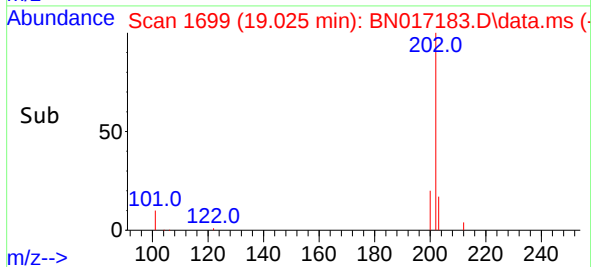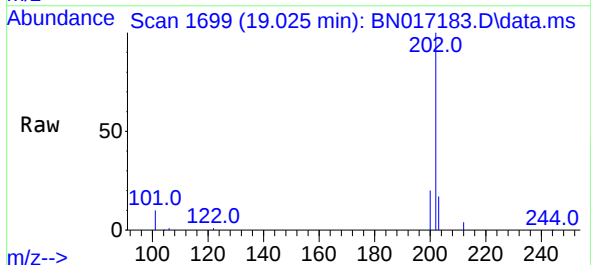



#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.165 min Scan# 2006

Delta R.T. 0.000 min

Lab File: BN017183.D

Acq: 29 Oct 2021 16:51





Tgt Ion:240 Resp: 138952

Ion Ratio Lower Upper

240 100

120 6.2 5.0 7.4

236 25.4 20.3 30.5

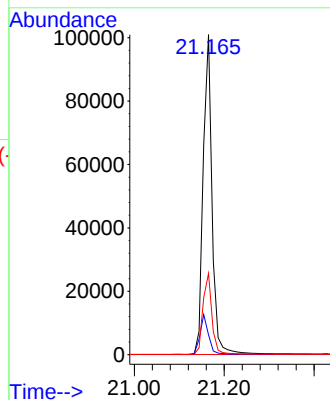

#30

Pyrene

Concen: 0.372 ng

RT: 19.392 min Scan# 1773

Delta R.T. 0.000 min

Lab File: BN017183.D

Acq: 29 Oct 2021 16:51




Tgt Ion:202 Resp: 163050


Ion Ratio Lower Upper

202 100

200 20.6 16.5 24.7

203 17.5 14.0 21.0

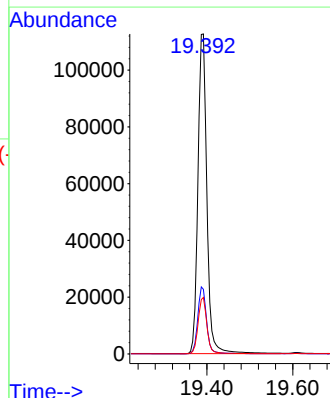







#31
 Terphenyl-d14
 Concen: 0.365 ng
 RT: 19.610 min Scan# 1817
 Delta R.T. 0.000 min
 Lab File: BN017183.D
 Acq: 29 Oct 2021 16:51

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.4

Tgt Ion:244 Resp: 112322




Ion	Ratio	Lower	Upper
244	100		
212	7.2	5.8	8.6
122	11.5	9.2	13.8

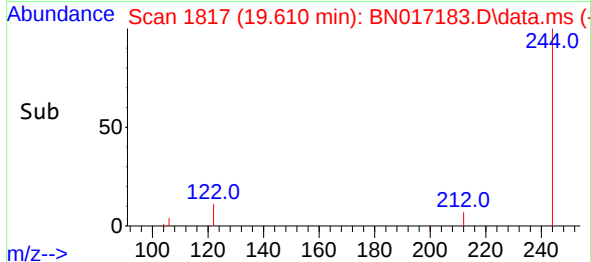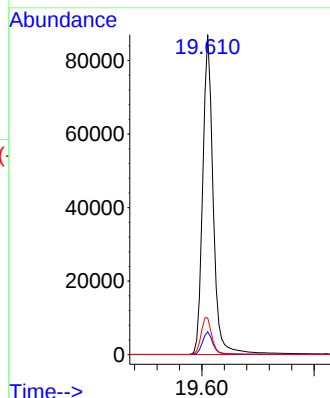


#32
 Benzo(a)anthracene
 Concen: 0.360 ng
 RT: 21.144 min Scan# 2004
 Delta R.T. 0.000 min
 Lab File: BN017183.D
 Acq: 29 Oct 2021 16:51

Tgt Ion:228 Resp: 147813

Ion	Ratio	Lower	Upper
228	100		
226	27.4	21.9	32.9
229	19.3	15.4	23.2

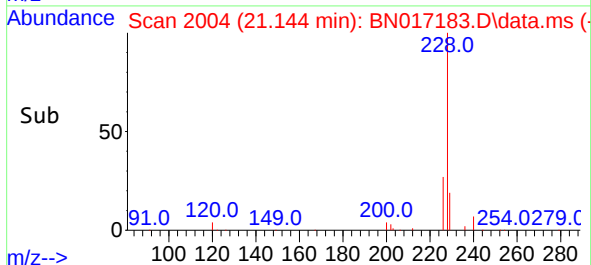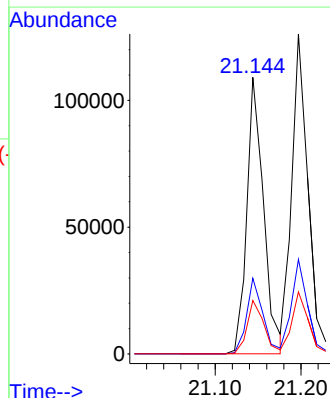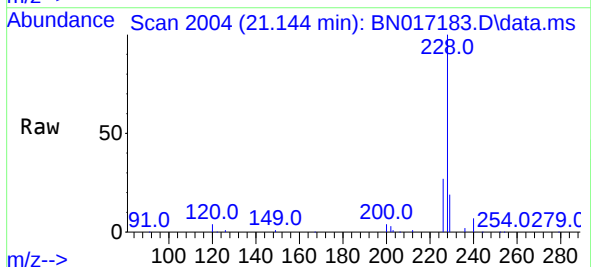







#33
Chrysene
Concen: 0.367 ng
RT: 21.197 min Scan# 2009
Delta R.T. 0.000 min
Lab File: BN017183.D
Acq: 29 Oct 2021 16:51

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

Tgt Ion:228 Resp: 165808




Ion	Ratio	Lower	Upper
228	100		
226	29.5	23.6	35.4
229	19.4	15.5	23.3

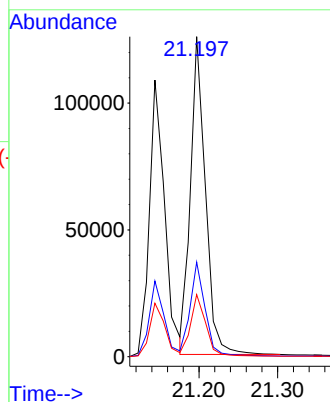


#34
Bis(2-ethylhexyl)phthalate
Concen: 0.271 ng
RT: 21.101 min Scan# 2000
Delta R.T. 0.000 min
Lab File: BN017183.D
Acq: 29 Oct 2021 16:51

Tgt Ion:149 Resp: 48088


Ion	Ratio	Lower	Upper
149	100		
167	27.0	21.6	32.4
279	4.0	3.2	4.8

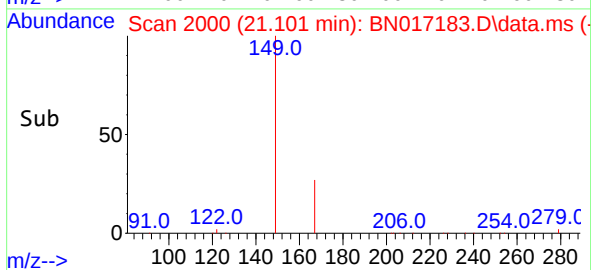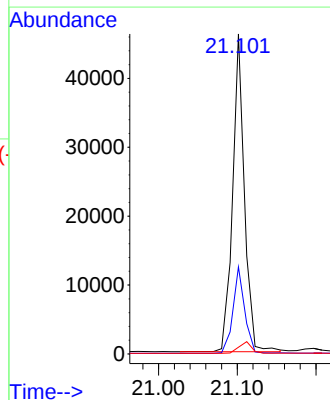





#35
Perylene-d12
Concen: 0.400 ng
RT: 23.376 min Scan# 2406
Delta R.T. 0.000 min
Lab File: BN017183.D
Acq: 29 Oct 2021 16:51


Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4





Tgt Ion:264 Resp: 137350
Ion Ratio Lower Upper
264 100
260 24.2 19.4 29.0
265 22.8 18.2 27.4




#36
Indeno(1,2,3-cd)pyrene
Concen: 0.399 ng
RT: 25.598 min Scan# 3055
Delta R.T. 0.000 min
Lab File: BN017183.D
Acq: 29 Oct 2021 16:51

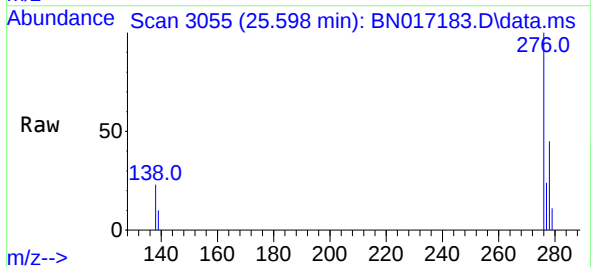

Tgt Ion:276 Resp: 186931
Ion Ratio Lower Upper
276 100
138 25.5 20.4 30.6
277 25.0 20.0 30.0

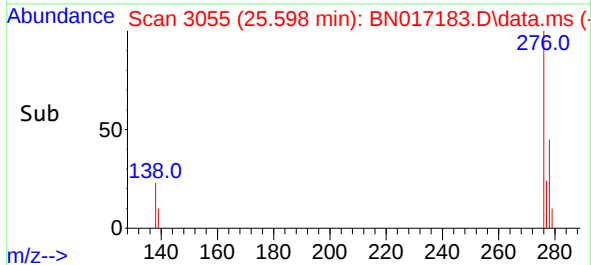



#37

Benzo(b)fluoranthene

Concen: 0.360 ng





RT: 22.712 min Scan# 2212

Delta R.T. 0.000 min

Lab File: BN017183.D

Acq: 29 Oct 2021 16:51

Tgt Ion:252	Resp:	161395
Ion	Ratio	Lower Upper
252	100	
253	21.9	17.5 26.3
125	9.9	7.9 11.9



#38

Benzo(k)fluoranthene

Concen: 0.365 ng




RT: 22.753 min Scan# 2224

Delta R.T. 0.000 min


Lab File: BN017183.D

Acq: 29 Oct 2021 16:51

Tgt Ion:252	Resp:	162581
Ion	Ratio	Lower Upper
252	100	
253	22.0	17.6 26.4
125	11.5	9.2 13.8

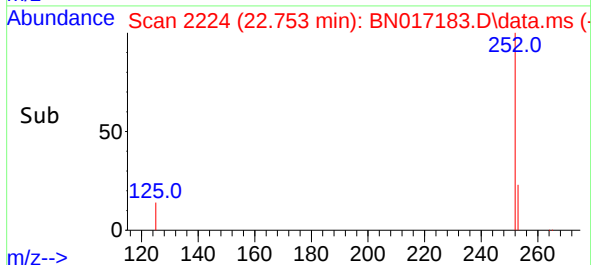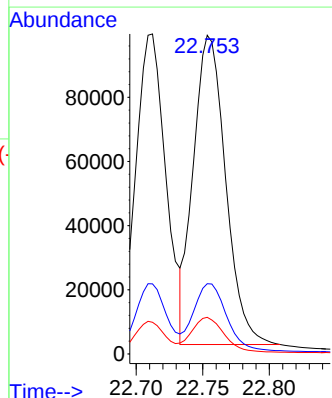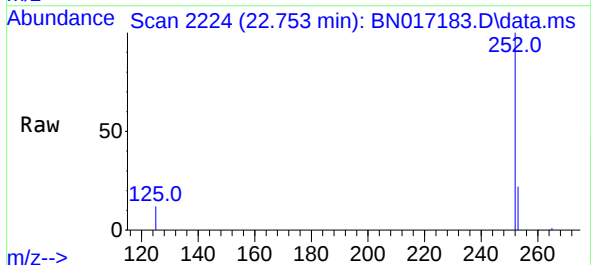





Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4



#39
Benzo(a)pyrene
Concen: 0.362 ng
RT: 23.274 min Scan# 2376
Delta R.T. 0.000 min
Lab File: BN017183.D
Acq: 29 Oct 2021 16:51




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:252 Resp: 141811
Ion Ratio Lower Upper
252 100
253 22.0 17.6 26.4
125 11.4 9.1 13.7

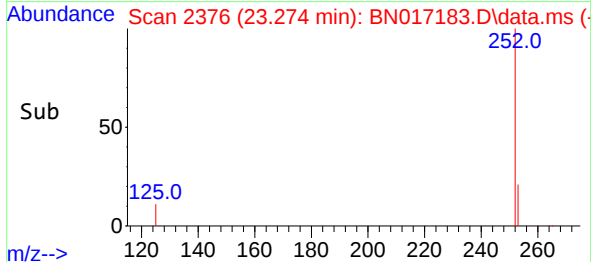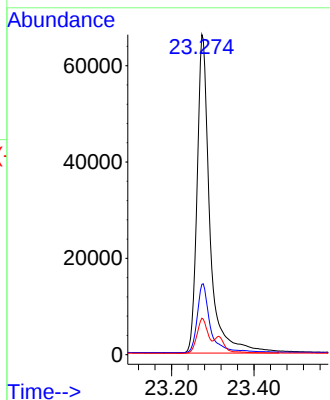

#40
Dibenzo(a,h)anthracene
Concen: 0.403 ng
RT: 25.622 min Scan# 3062
Delta R.T. 0.000 min
Lab File: BN017183.D
Acq: 29 Oct 2021 16:51

Tgt Ion:278 Resp: 151026
Ion Ratio Lower Upper
278 100
139 16.5 13.2 19.8
279 23.8 19.0 28.6

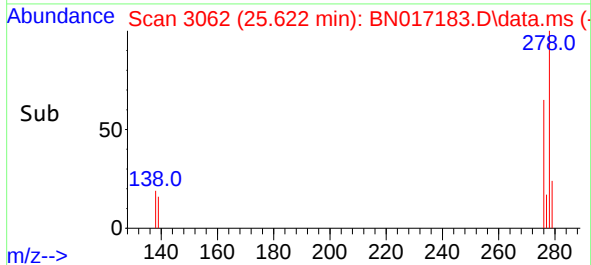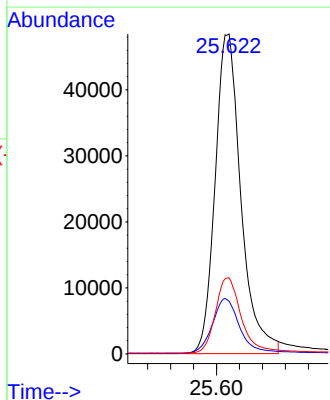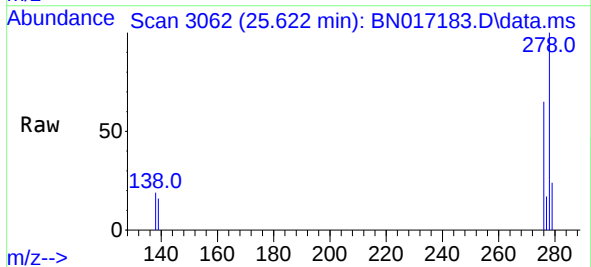

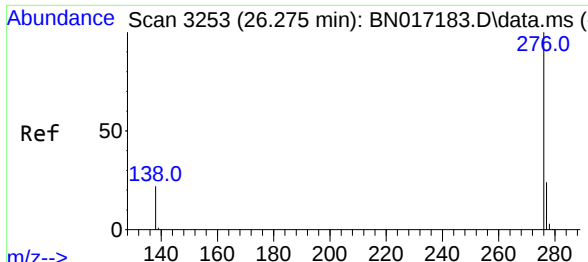

#41
Benzo(g,h,i)perylene
Concen: 0.393 ng
RT: 26.275 min Scan# 3253
Delta R.T. 0.000 min
Lab File: BN017183.D
Acq: 29 Oct 2021 16:51

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

Tgt Ion:276 Resp: 164255
Ion Ratio Lower Upper
276 100
277 23.7 19.0 28.4
138 21.7 17.4 26.0

