


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102921\
 Data File : BN017180.D
 Acq On : 29 Oct 2021 14:20
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN102921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Oct 30 00:49:11 2021

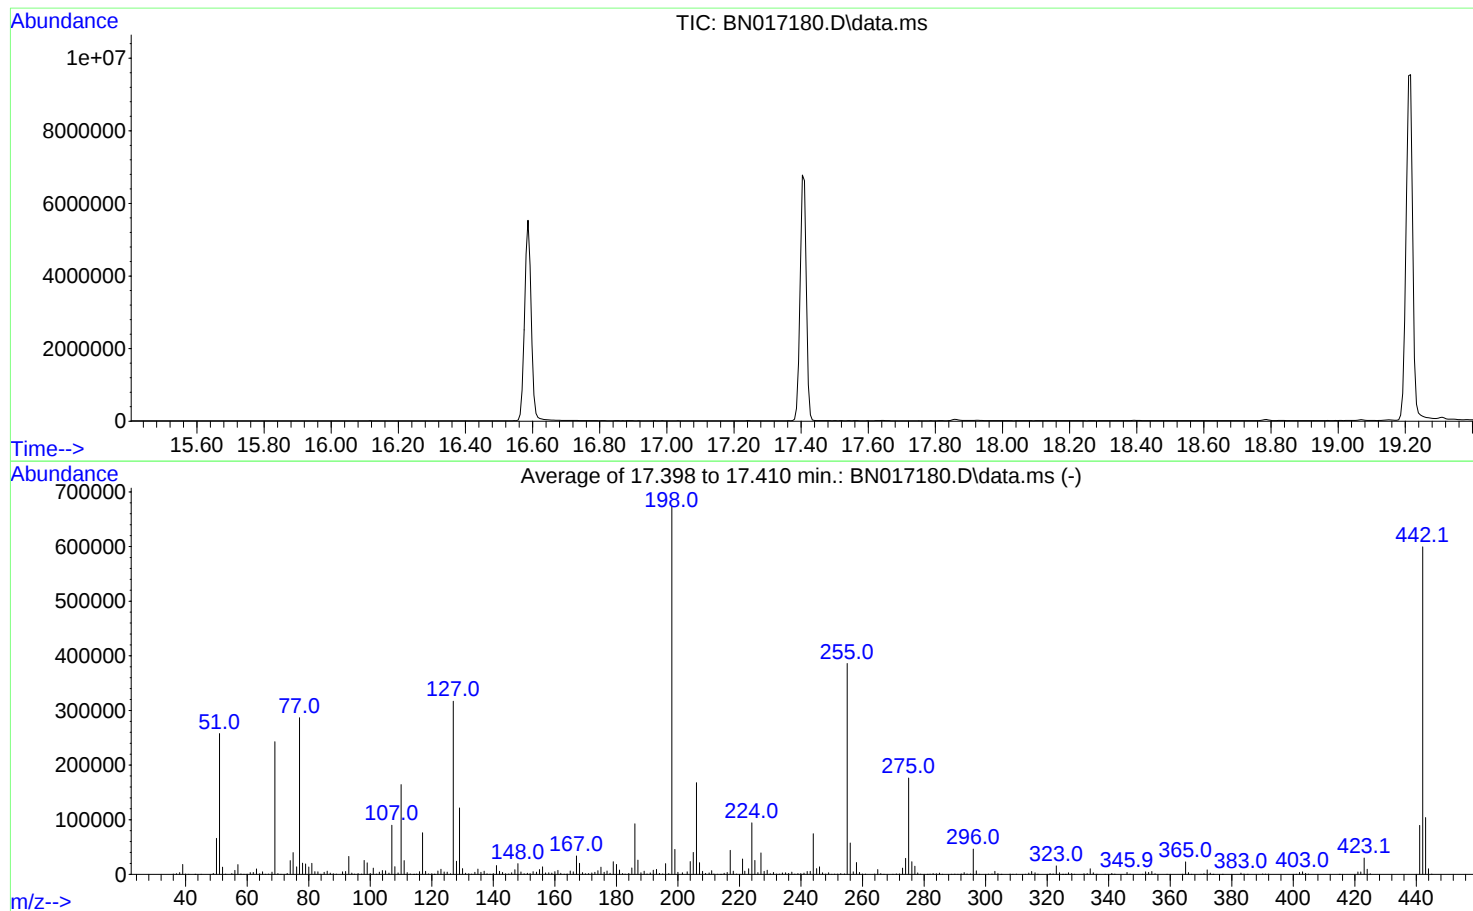




AutoFind: Scans 2450, 2451, 2452; Background Corrected with Scan 2443

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.3	257877	PASS
68	69	0.00	2	1.7	4079	PASS
69	198	0.00	100	36.1	242880	PASS
70	69	0.00	2	0.6	1361	PASS
127	198	10	80	47.1	317013	PASS
197	198	0.00	2	0.2	1420	PASS
198	198	100	100	100.0	673323	PASS
199	198	5	9	6.8	45747	PASS
275	198	10	60	26.2	176429	PASS
365	198	1	100	3.4	22874	PASS
441	198	0.01	100	13.3	89509	PASS
442	442	50	100	100.0	599445	PASS
443	442	15	24	17.4	104048	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102921\
 Data File : BN017180.D
 Acq On : 29 Oct 2021 14:20
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Oct 30 02:30:36 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Oct 30 02:30:31 2021
 Response via : Initial Calibration

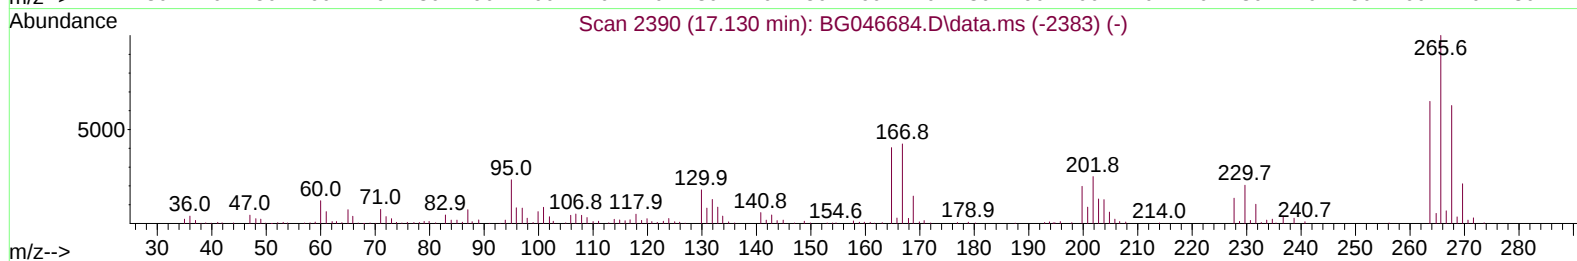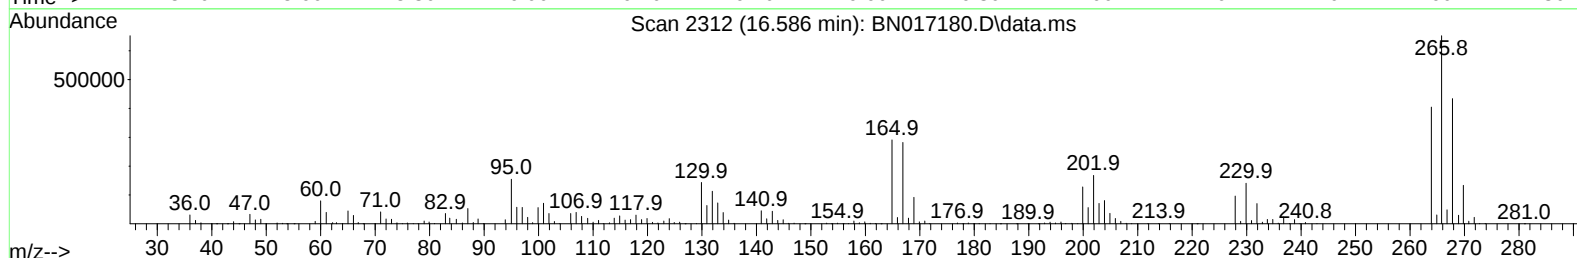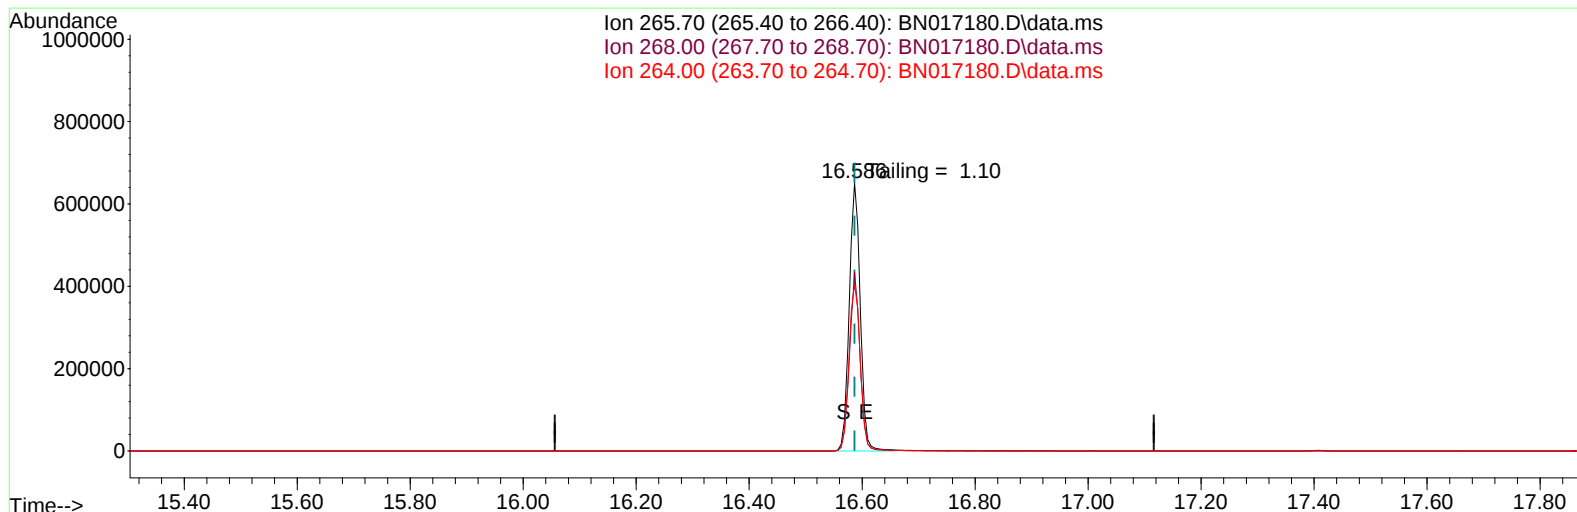

TIC: BN017180.D\data.ms

(70) Pentachlorophenol (C)

16.586min (0.000) 25111.71 ng




response 890167

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.59
264.00	61.60	62.08
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102921\
Data File : BN017180.D
Acq On : 29 Oct 2021 14:20
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 30 02:30:36 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 30 02:30:31 2021
Response via : Initial Calibration

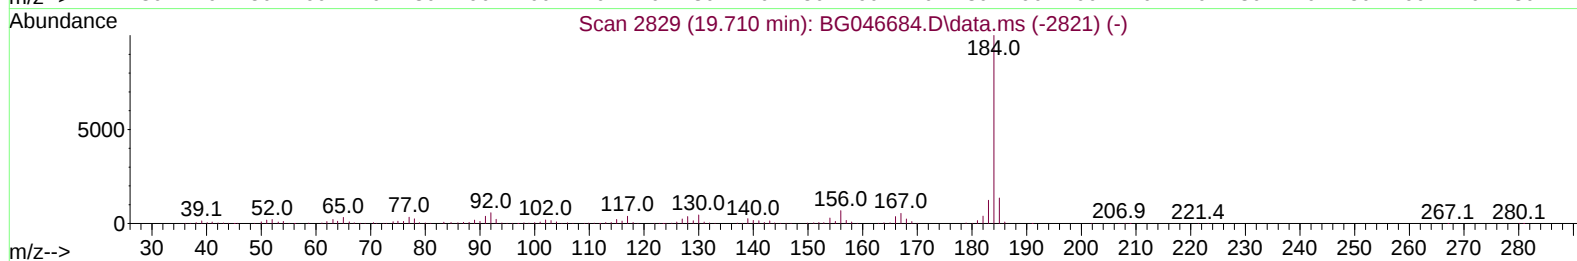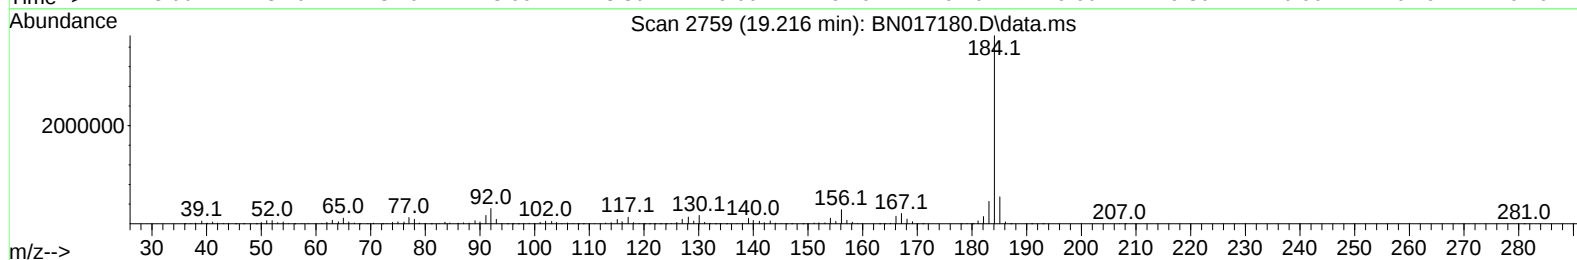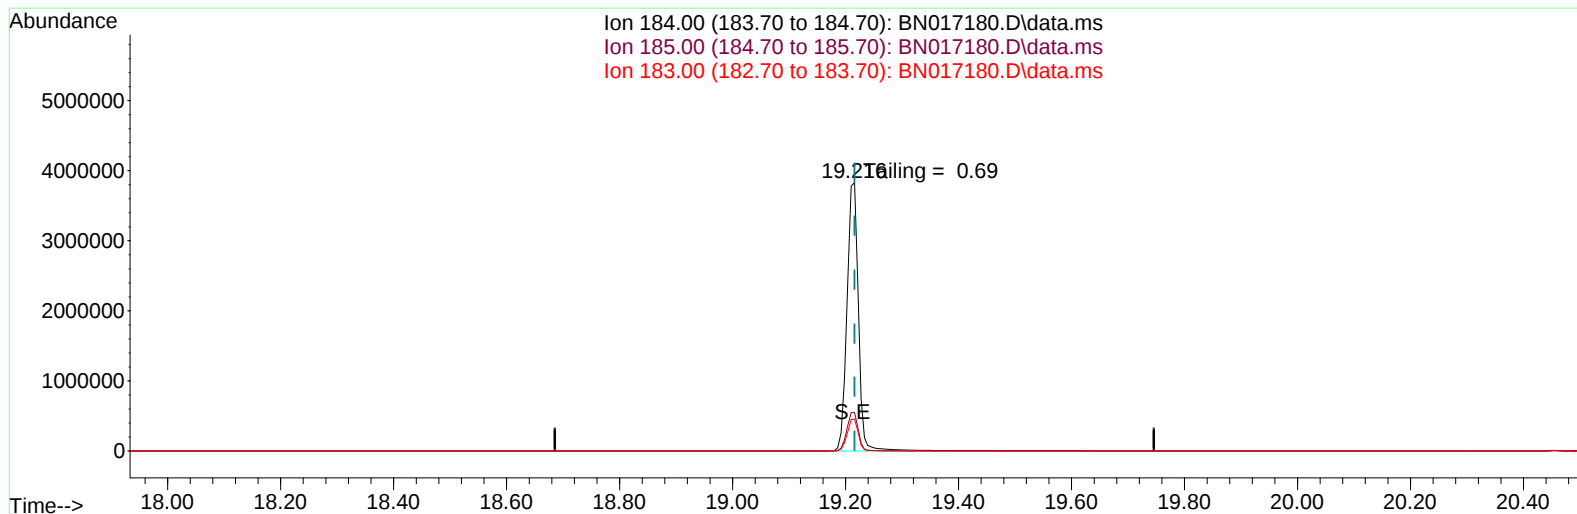

TIC: BN017180.D\data.ms

(77) Benzidine

19.216min (0.000) 0.00 ng

response 5403340

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.35
183.00	13.20	11.93
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/29/2021	BNA_N	<u>BN017180.D</u>
Compound Name	Response	Retention Time
DDT	2458339	20.457
DDD	11176	20.057
DDE	0	19.58
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11176	2469515	0.45

Instrument :
BNA_N
ClientSampleId :
DFTPP