


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103018\
 Data File : BN003355.D
 Acq On : 30 Oct 2018 11:28
 Operator : MJ/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN102618.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 29 16:15:49 2018

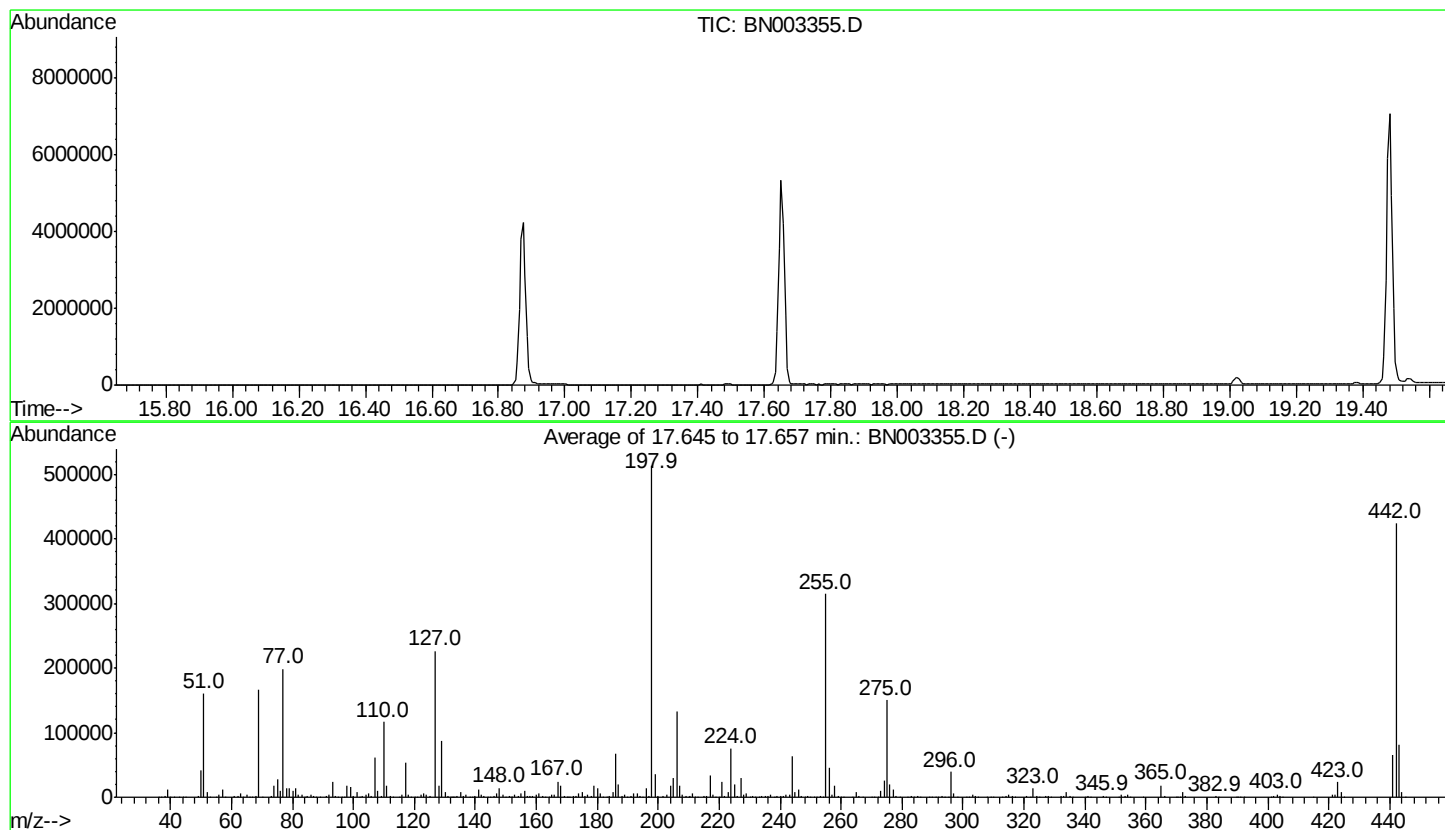

AutoFind: Scans 2492, 2493, 2494; Background Corrected with Scan 2485

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.2	160178	PASS
68	69	0.00	2	1.8	2943	PASS
69	198	0.00	100	32.3	165760	PASS
70	69	0.00	2	0.5	876	PASS
127	198	10	80	44.0	225941	PASS
197	198	0.00	2	0.4	2006	PASS
198	198	100	100	100.0	513173	PASS
199	198	5	9	6.9	35474	PASS
275	198	10	60	29.3	150232	PASS
365	198	1	100	3.5	18103	PASS
441	198	0.01	100	12.7	65125	PASS
442	198	50	100	82.6	423680	PASS
443	442	15	24	19.2	81557	PASS