
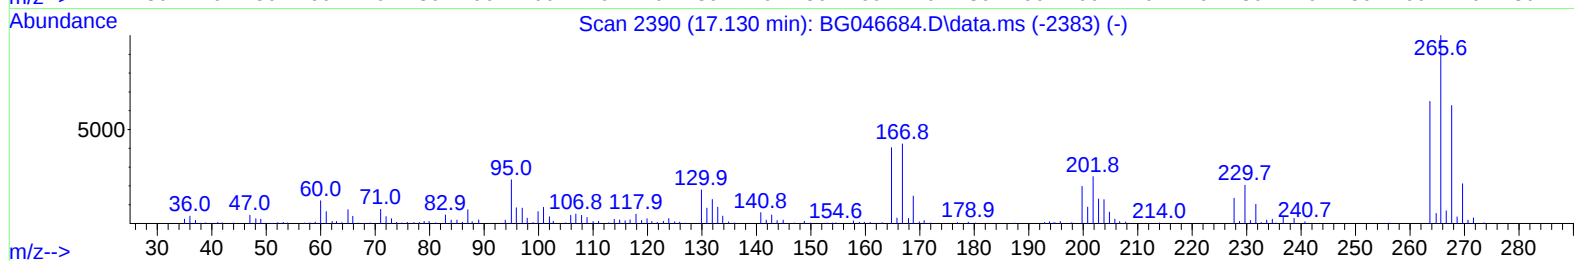
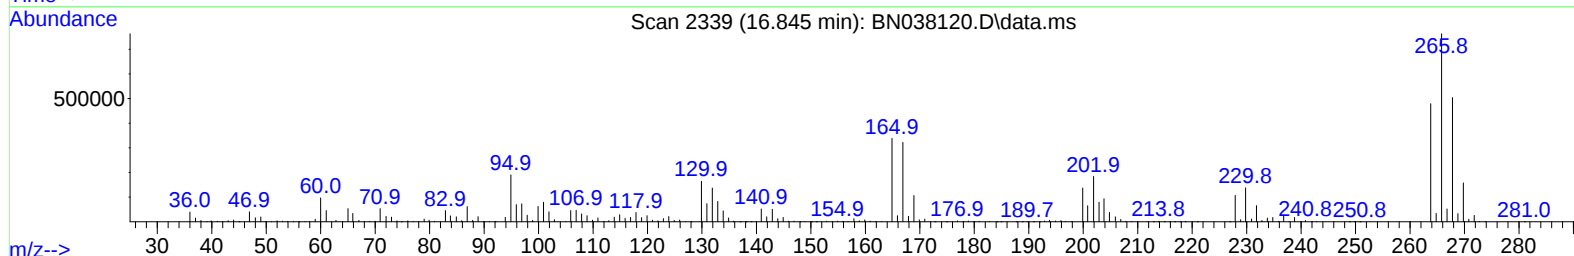


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103025\
Data File : BN038120.D
Acq On : 30 Oct 2025 09:21
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 30 11:03:28 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 30 11:03:15 2025
Response via : Initial Calibration

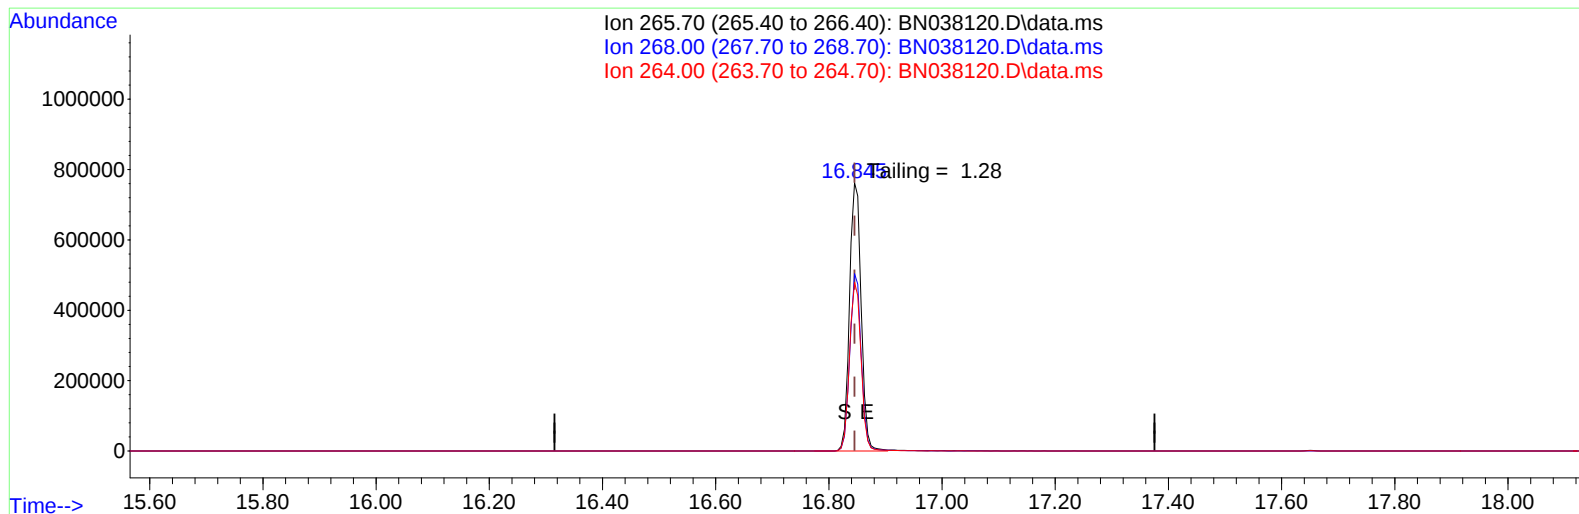

TIC: BN038120.D\data.ms

(70) Pentachlorophenol (C)




16.845min (0.000) 277.91 ng

response 1092521

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.05
264.00	61.60	62.83
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103025\
Data File : BN038120.D
Acq On : 30 Oct 2025 09:21
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 30 11:03:28 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 30 11:03:15 2025
Response via : Initial Calibration

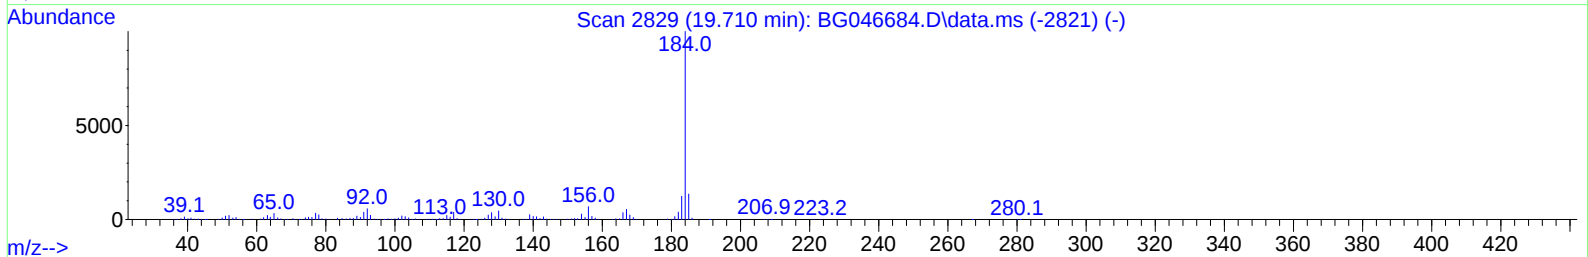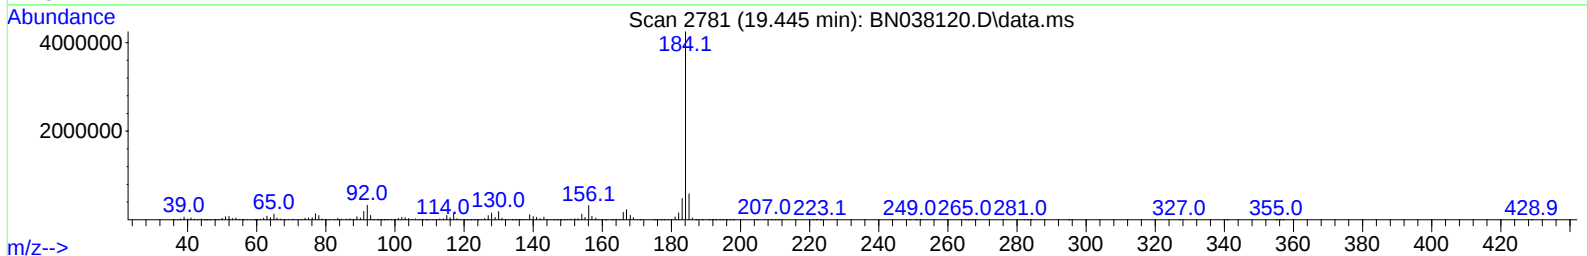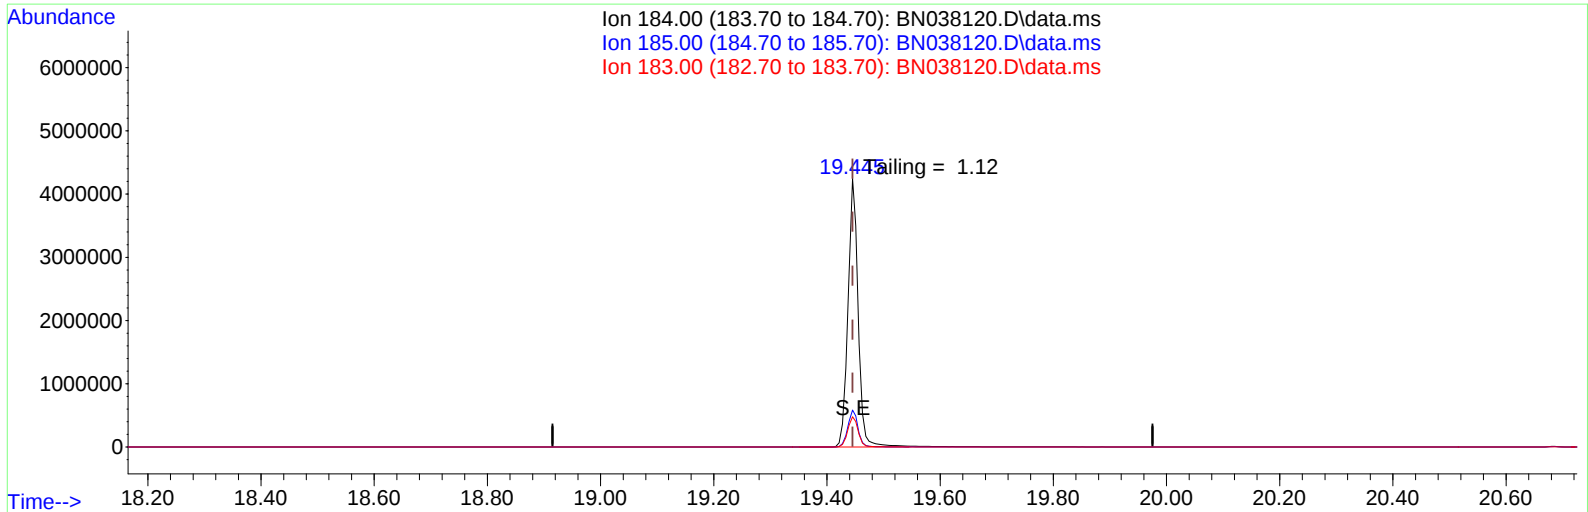

TIC: BN038120.D\data.ms

(77) Benzidine

19.445min (0.000) 0.00 ng

response 5317002

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.82
183.00	13.20	11.31
0.00	0.00	0.00