


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103025\
Data File : BN038120.D
Acq On : 30 Oct 2025 09:21
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN102825.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Oct 29 13:09:46 2025

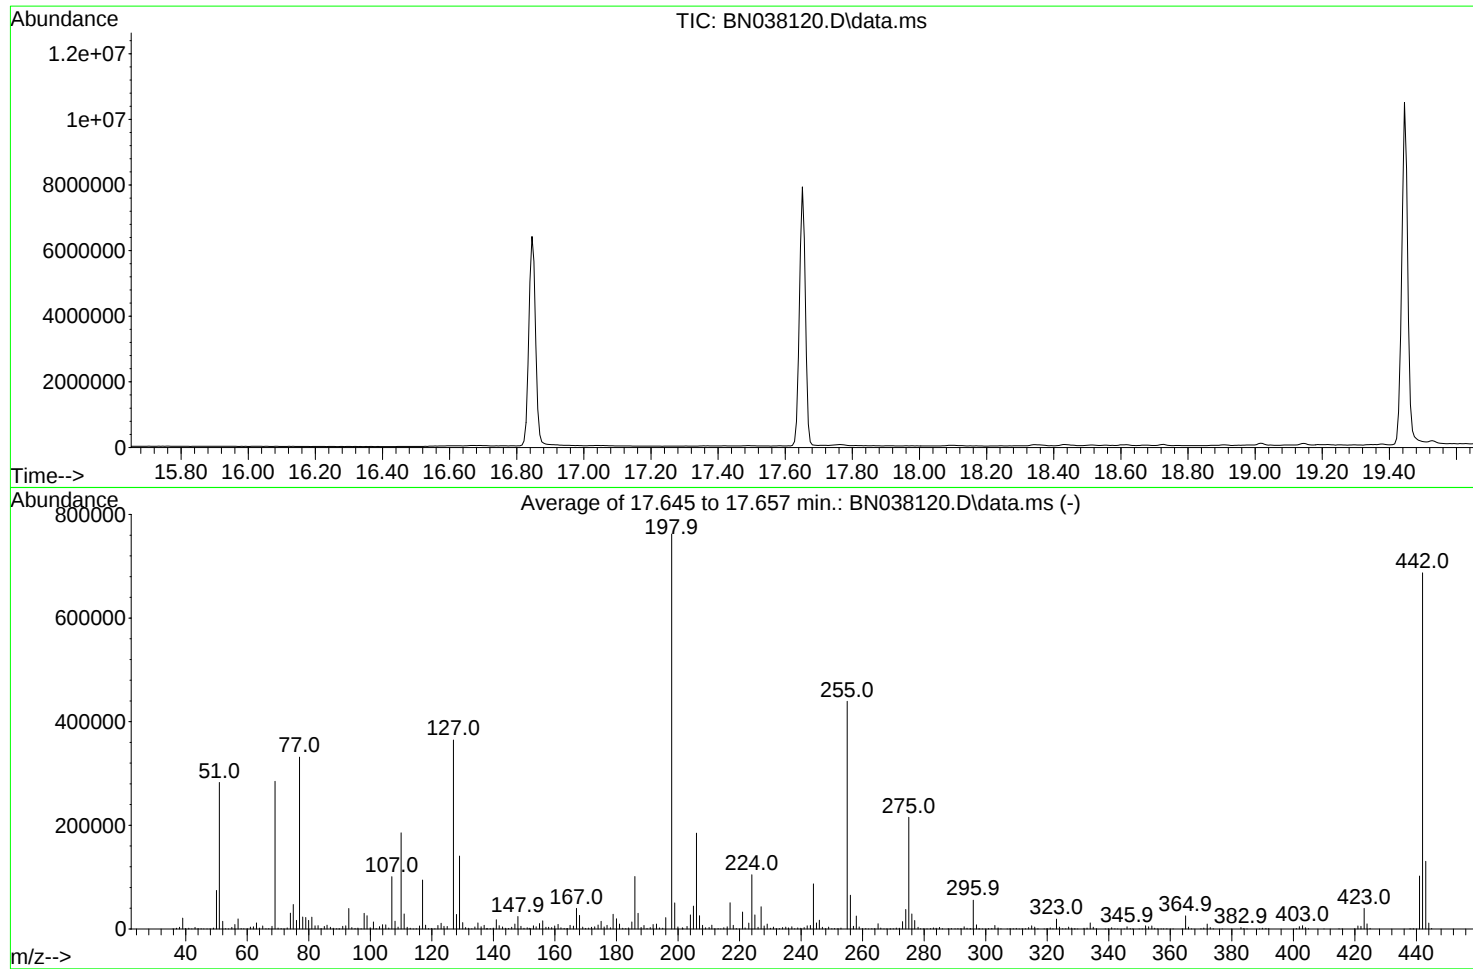




AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2468

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.8	5144	PASS
69	69	100	100	100.0	284922	PASS
70	69	0.00	2	0.6	1800	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	762155	PASS
199	198	5	9	6.6	50232	PASS
365	198	1	100	3.3	25341	PASS
441	443	0.01	150	78.2	101981	PASS
442	442	100	100	100.0	687317	PASS
443	442	15	24	19.0	130451	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103025\
Data File : BN038120.D
Acq On : 30 Oct 2025 09:21
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 30 11:03:28 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 30 11:03:15 2025
Response via : Initial Calibration

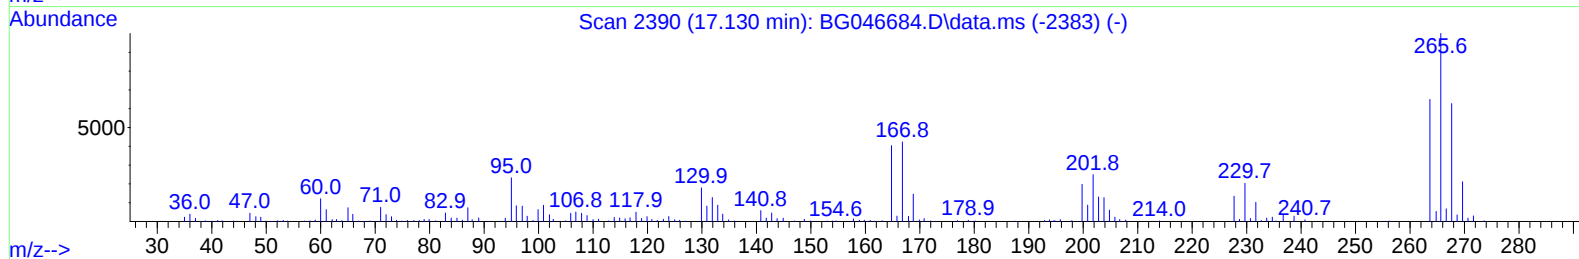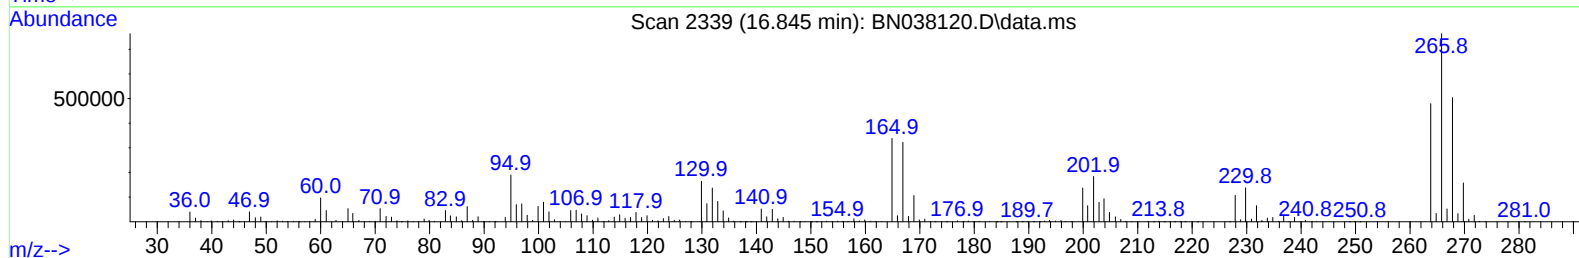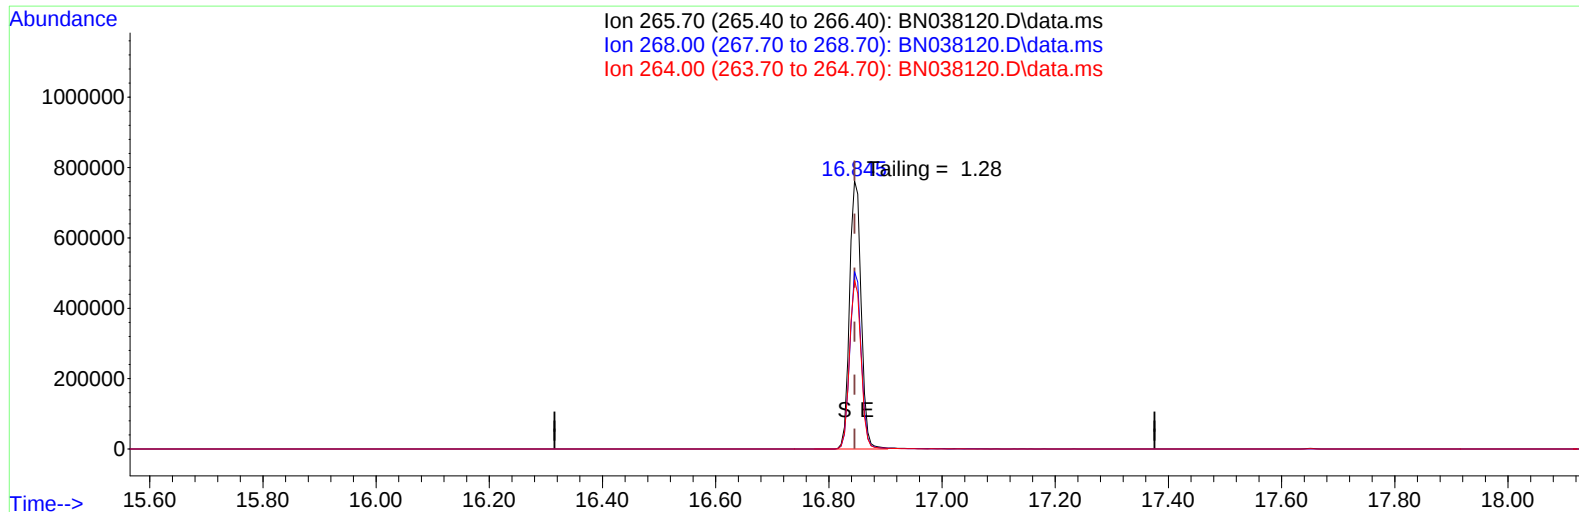

TIC: BN038120.D\data.ms

(70) Pentachlorophenol (C)

16.845min (0.000) 277.91 ng




response 1092521

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.05
264.00	61.60	62.83
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103025\
Data File : BN038120.D
Acq On : 30 Oct 2025 09:21
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 30 11:03:28 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 30 11:03:15 2025
Response via : Initial Calibration

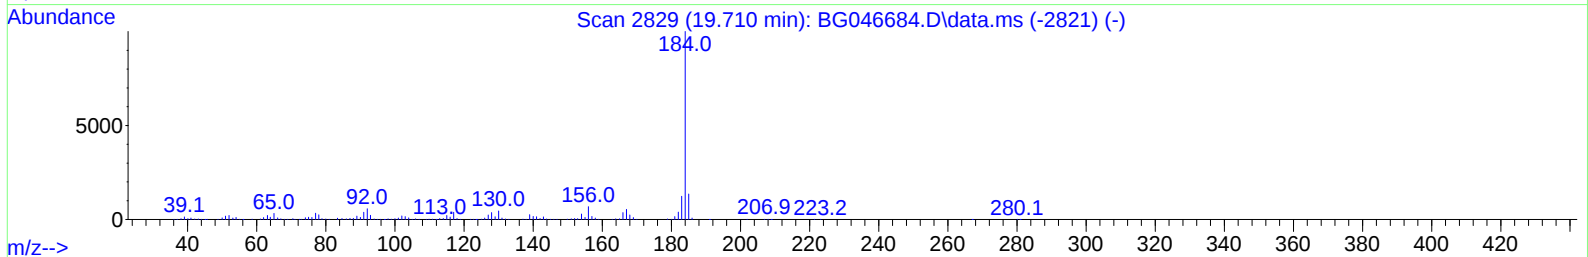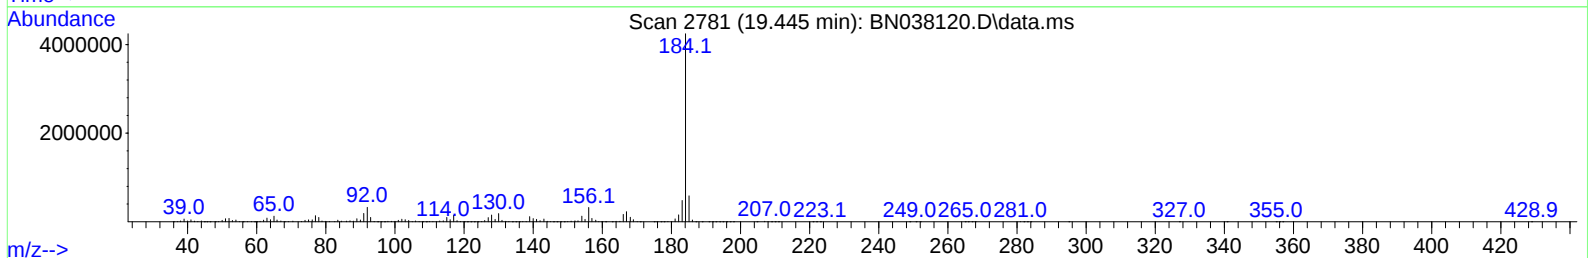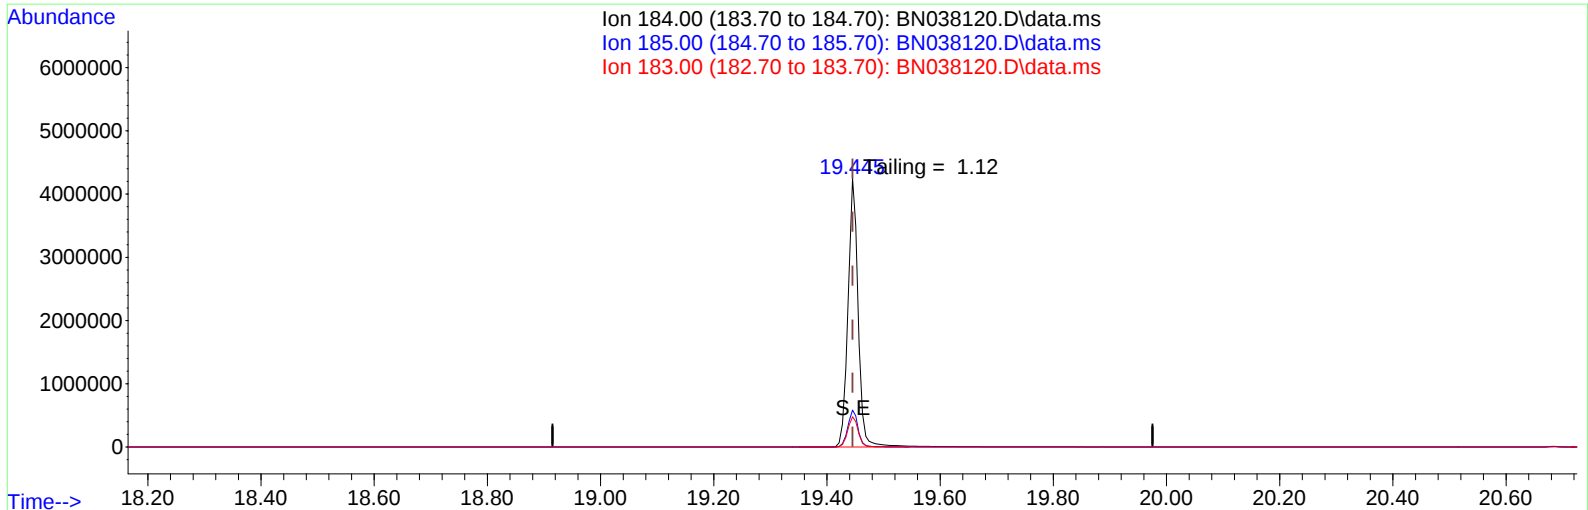

TIC: BN038120.D\data.ms

(77) Benzidine

19.445min (0.000) 0.00 ng

response 5317002

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.82
183.00	13.20	11.31
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/30/2025	BNA_N	<u>BN038120.D</u>
Compound Name	Response	Retention Time
DDT	2793166	20.686
DDD	20273	20.245
DDE	1753	19.739
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
22026	2815192	0.78

Instrument :
BNA_N
ClientSampleId :
DFTPP