


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103118\
 Data File : BN003365.D
 Acq On : 31 Oct 2018 09:55
 Operator : MJ/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN102618.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 29 16:15:49 2018

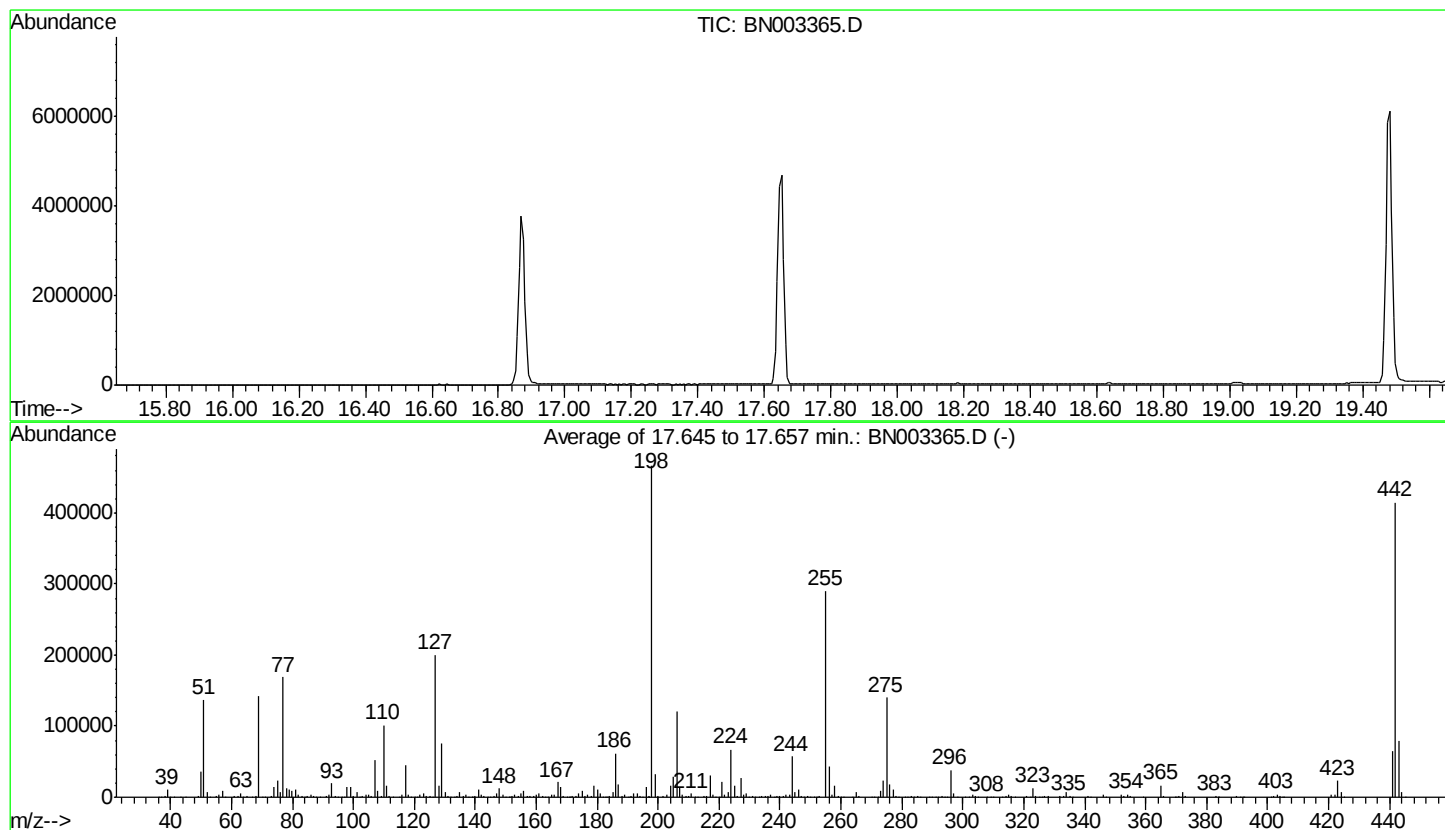

AutoFind: Scans 2492, 2493, 2494; Background Corrected with Scan 2485

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.4	137146	PASS
68	69	0.00	2	1.8	2513	PASS
69	198	0.00	100	30.7	143056	PASS
70	69	0.00	2	0.6	841	PASS
127	198	10	80	43.0	200322	PASS
197	198	0.00	2	0.4	1913	PASS
198	198	100	100	100.0	466368	PASS
199	198	5	9	6.8	31712	PASS
275	198	10	60	29.9	139645	PASS
365	198	1	100	3.6	17002	PASS
441	198	0.01	100	13.8	64392	PASS
442	198	50	100	88.8	414336	PASS
443	442	15	24	19.2	79674	PASS