
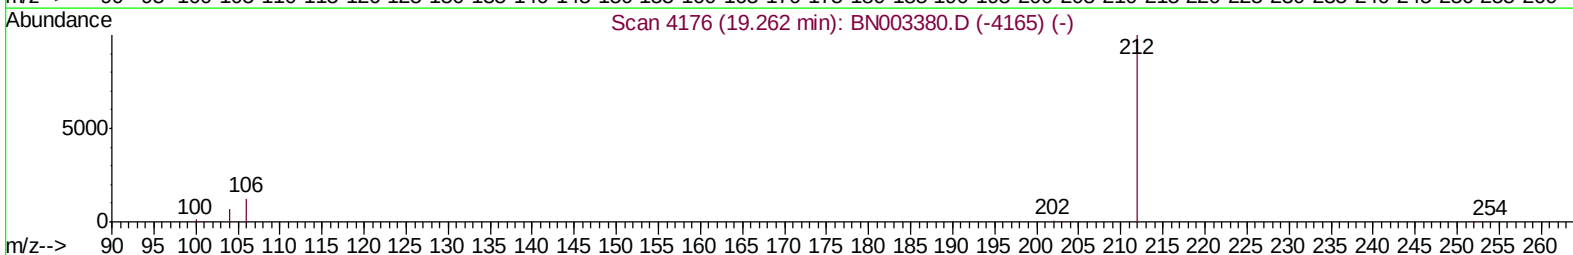
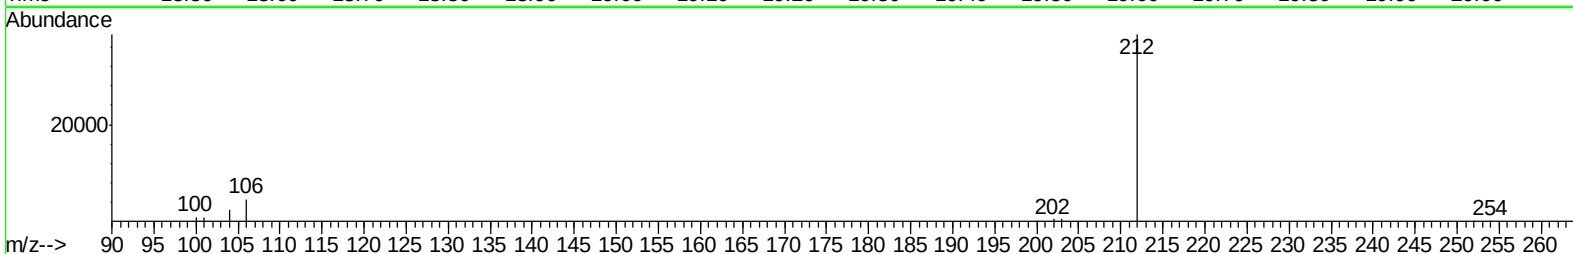


Data File : BN003384.D  
Acq On : 01 Nov 2018 18:24  
Operator : MJ/SJ  
Sample : J5657-16  
Misc :  
ALS Vial : 15 Sample Multiplier: 1

Quant Time: Nov 02 04:55:38 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\SOM-EPA-SIM-BN110118.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Nov 02 04:49:17 2018  
Response via : Initial Calibration

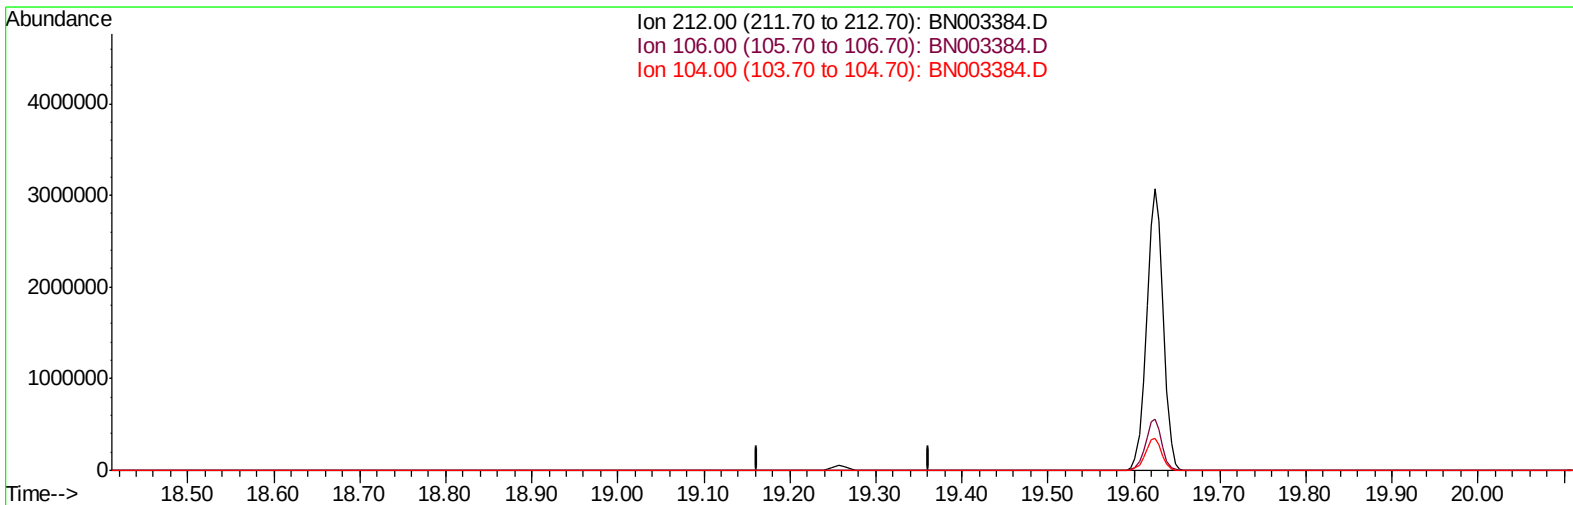

TIC: BN003384.D

(14) Fluoranthene-d10 (SURR)

19.262min (-19.262) 0.00ng/ul

response 0

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 212.00 | 100   | 0.00  |
| 106.00 | 13.50 | 0.00# |
| 104.00 | 7.60  | 0.00# |
| 0.00   | 0.00  | 0.00  |