
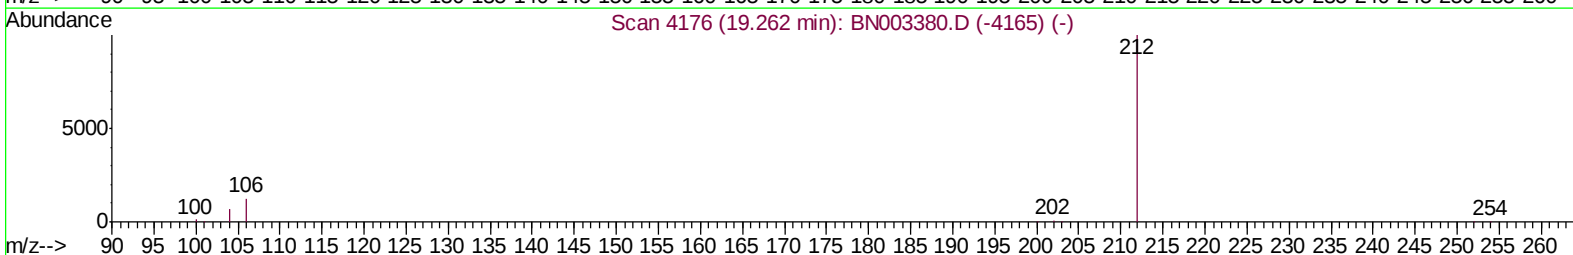
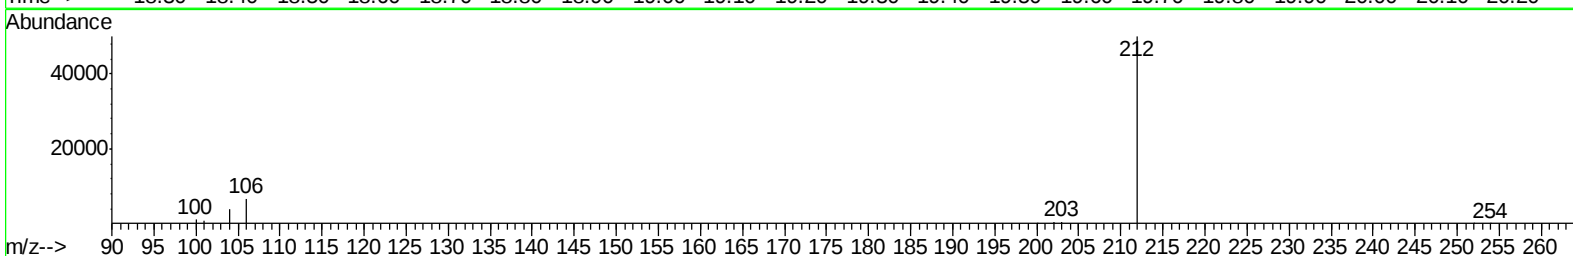


Data File : BN003384.D
Acq On : 01 Nov 2018 18:24
Operator : MJ/SJ
Sample : J5657-16
Misc :
ALS Vial : 15 Sample Multiplier: 1

Quant Time: Nov 02 04:55:38 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 02 04:49:17 2018
Response via : Initial Calibration

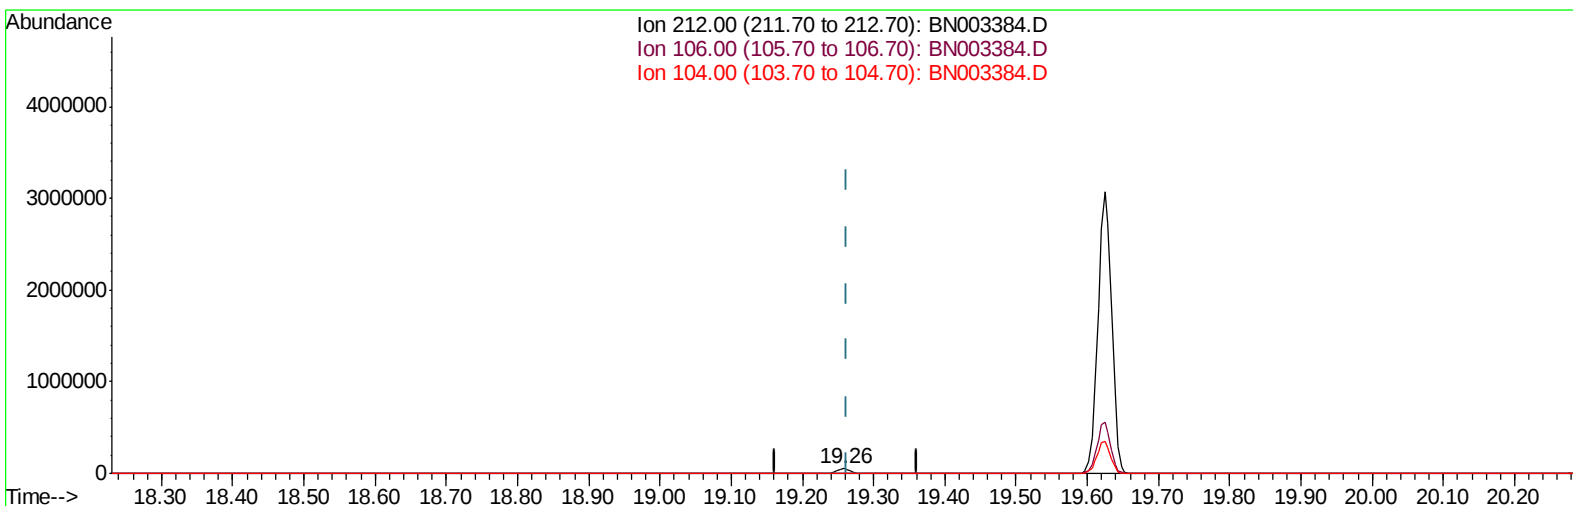

TIC: BN003384.D

(14) Fluoranthene-d10 (SURR)

19.258min (-0.005) 0.35ng/ul m

response 64804

Ion	Exp%	Act%
212.00	100	100
106.00	13.50	0.00#
104.00	7.60	0.00#
0.00	0.00	0.00