
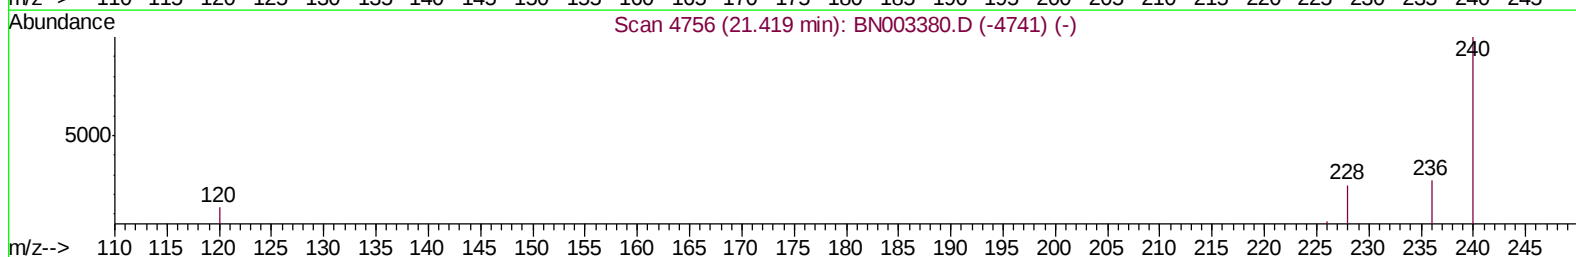
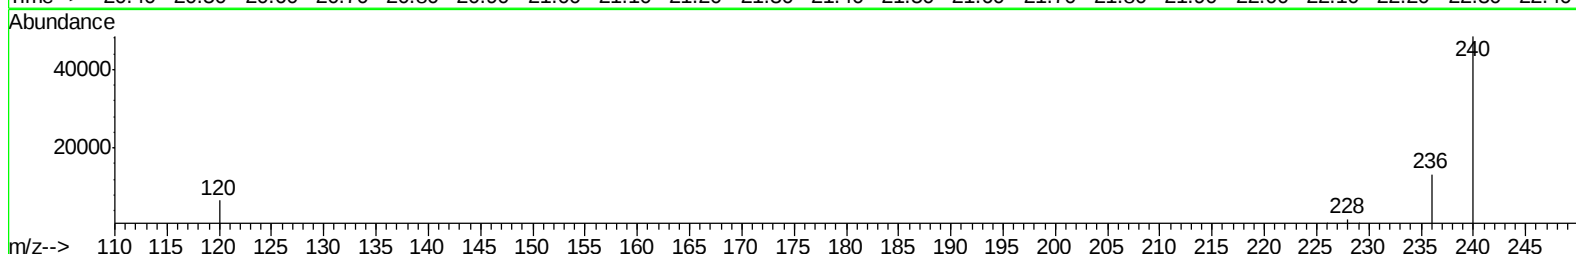


Data File : BN003384.D
Acq On : 01 Nov 2018 18:24
Operator : MJ/SJ
Sample : J5657-16
Misc :
ALS Vial : 15 Sample Multiplier: 1

Quant Time: Nov 02 04:55:38 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 02 04:49:17 2018
Response via : Initial Calibration

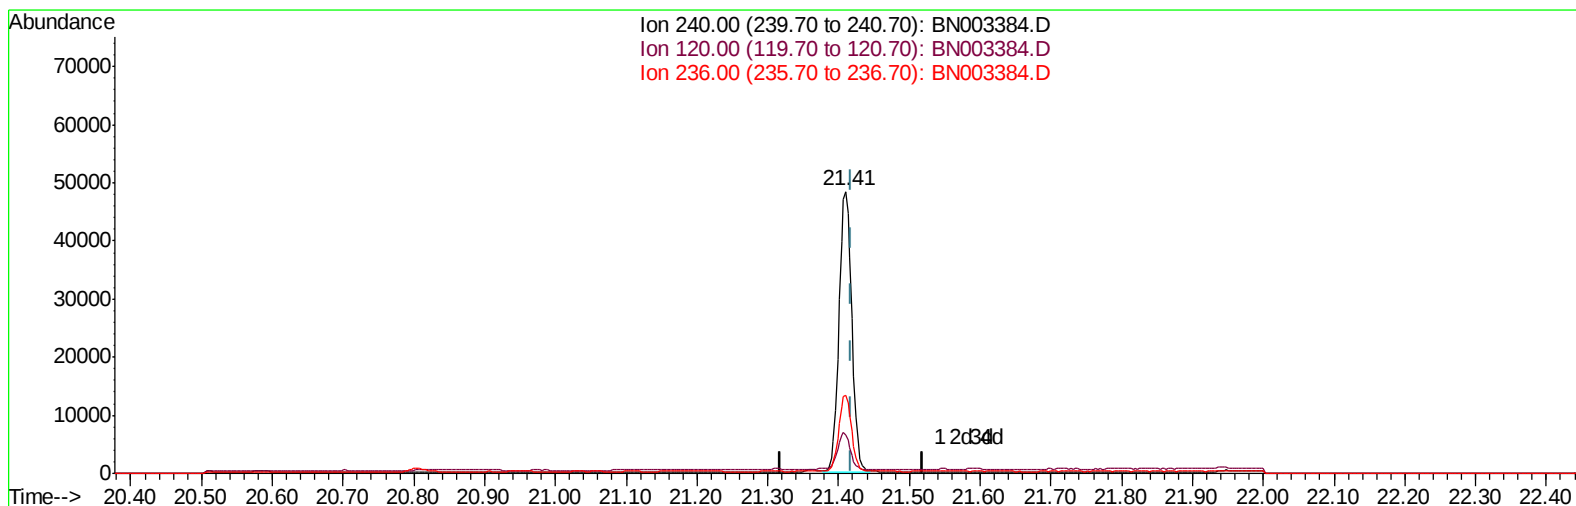

TIC: BN003384.D

(16) Chrysene-d12 (I)

21.410min (-0.009) 0.40ng/ul m

response 60671

Ion	Exp%	Act%
240.00	100	100
120.00	13.80	13.79
236.00	27.60	27.58
0.00	0.00	0.00