
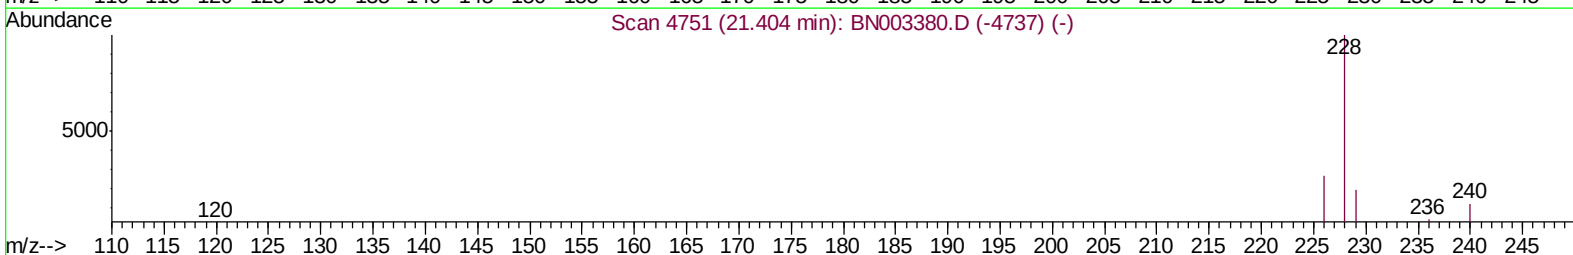
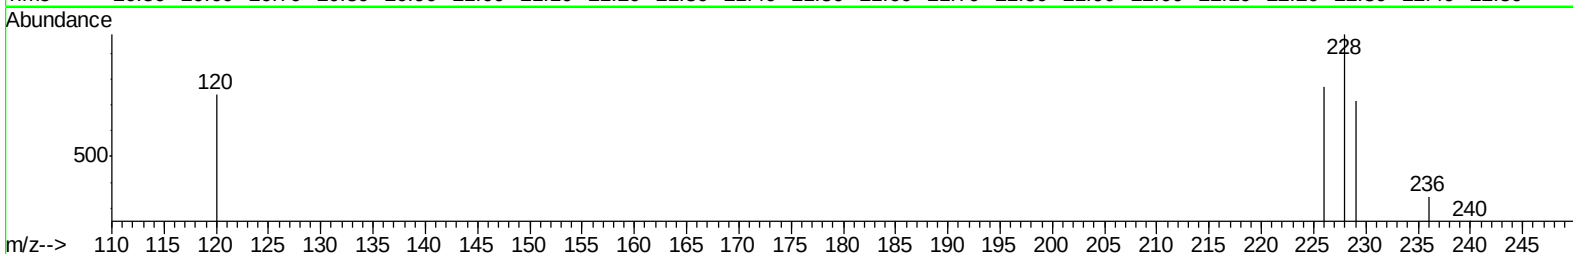


Data File : BN003384.D
Acq On : 01 Nov 2018 18:24
Operator : MJ/SJ
Sample : J5657-16
Misc :
ALS Vial : 15 Sample Multiplier: 1

Quant Time: Nov 02 04:57:20 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 02 04:49:17 2018
Response via : Initial Calibration

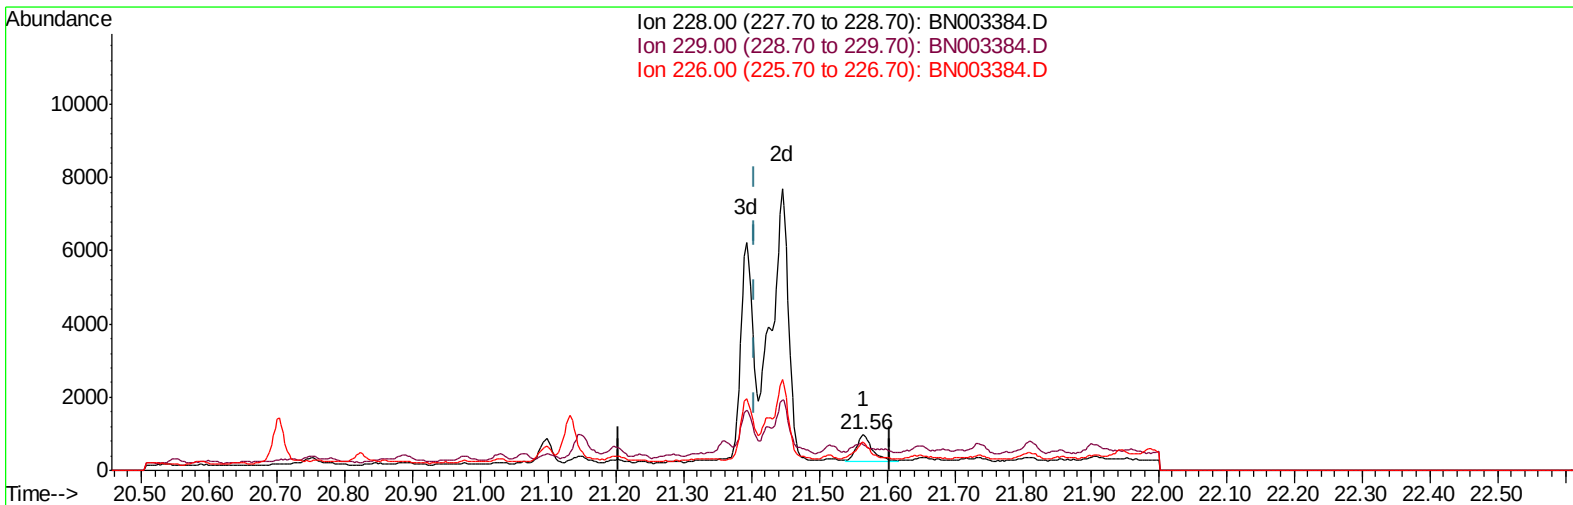

TIC: BN003384.D

(18) Benzo(a)anthracene
21.565min (+0.161) 0.01ng/ul
response 1124

Ion	Exp%	Act%
228.00	100	100
229.00	19.40	73.56#
226.00	26.90	79.12#
0.00	0.00	0.00