
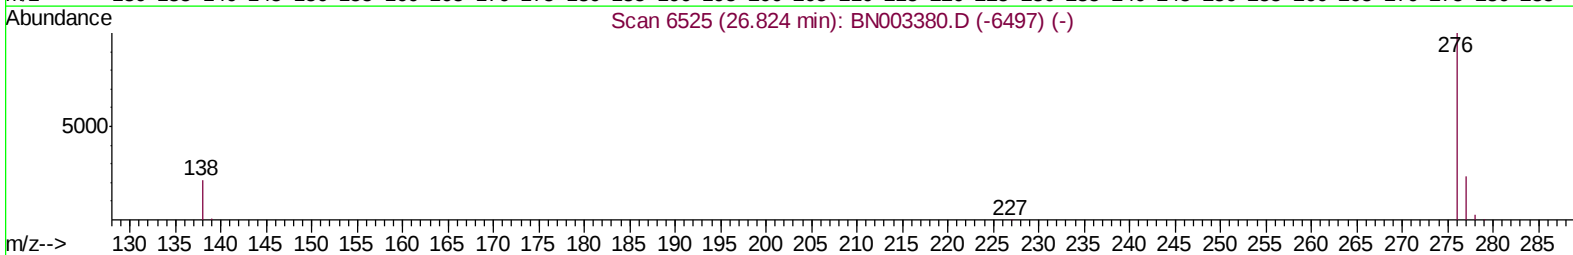
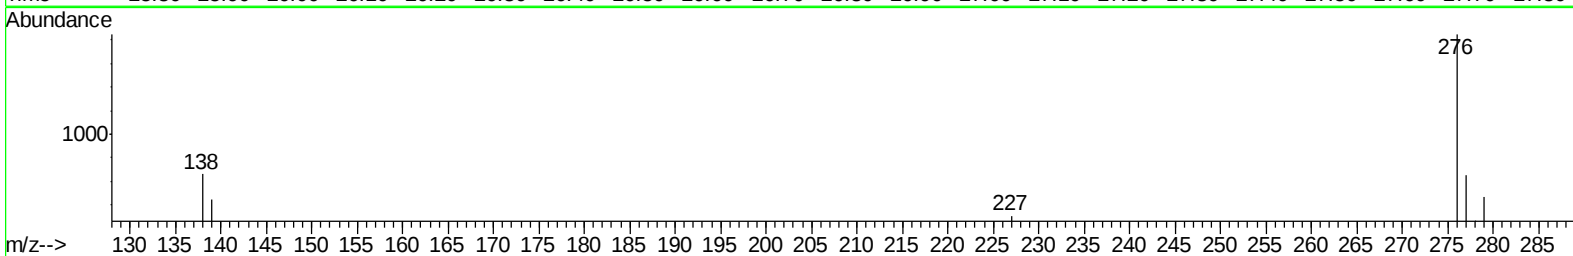


Data File : BN003384.D
Acq On : 01 Nov 2018 18:24
Operator : MJ/SJ
Sample : J5657-16
Misc :
ALS Vial : 15 Sample Multiplier: 1

Quant Time: Nov 02 05:00:59 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 02 04:49:17 2018
Response via : Initial Calibration

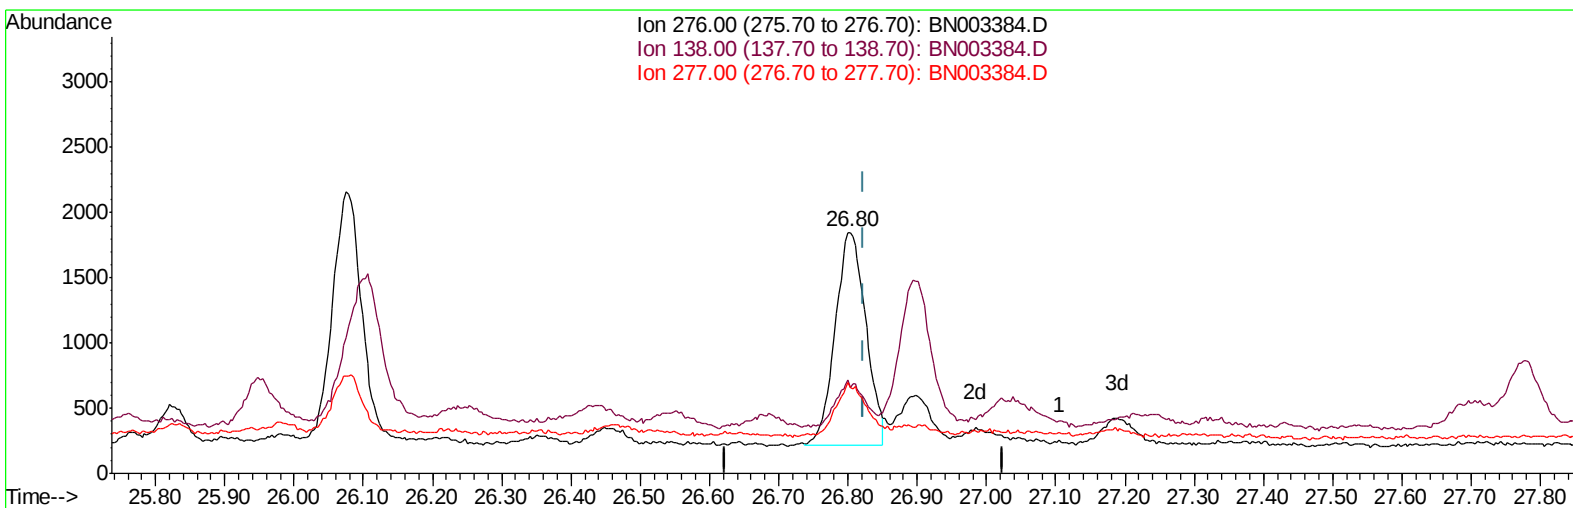

TIC: BN003384.D

(26) Benzo(g,h,i)perylene

26.803min (-0.020) 0.03ng/ul m

response 5020

Ion	Exp%	Act%
276.00	100	100
138.00	21.30	35.61#
277.00	24.00	35.50#
0.00	0.00	0.00