
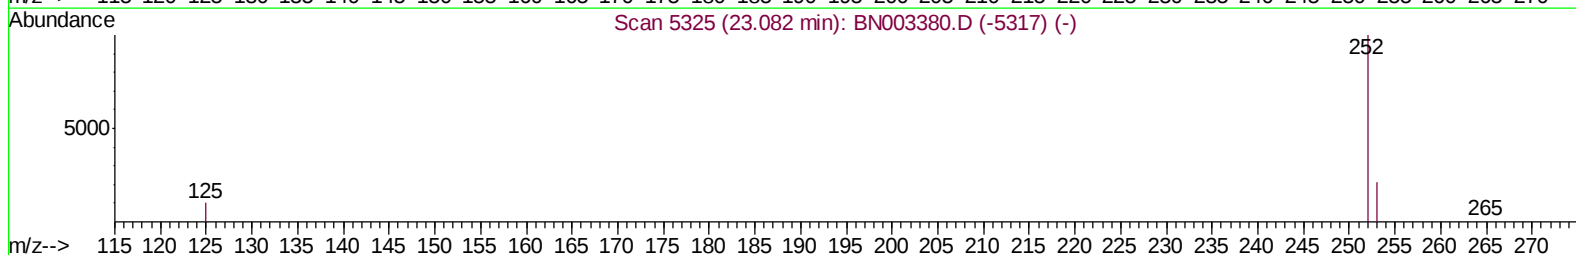
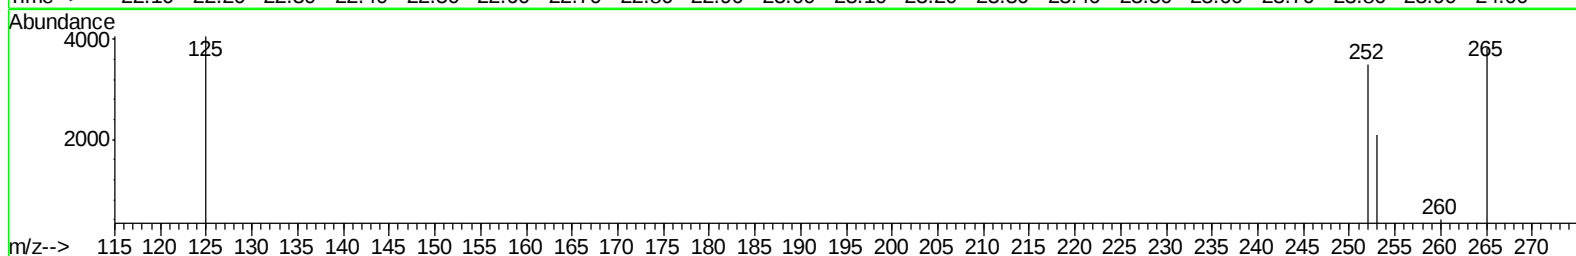


Data File : BN003385.D
Acq On : 01 Nov 2018 18:59
Operator : MJ/SJ
Sample : J5657-17MS
Misc :
ALS Vial : 16 Sample Multiplier: 1

Quant Time: Nov 02 04:52:03 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 02 04:49:17 2018
Response via : Initial Calibration

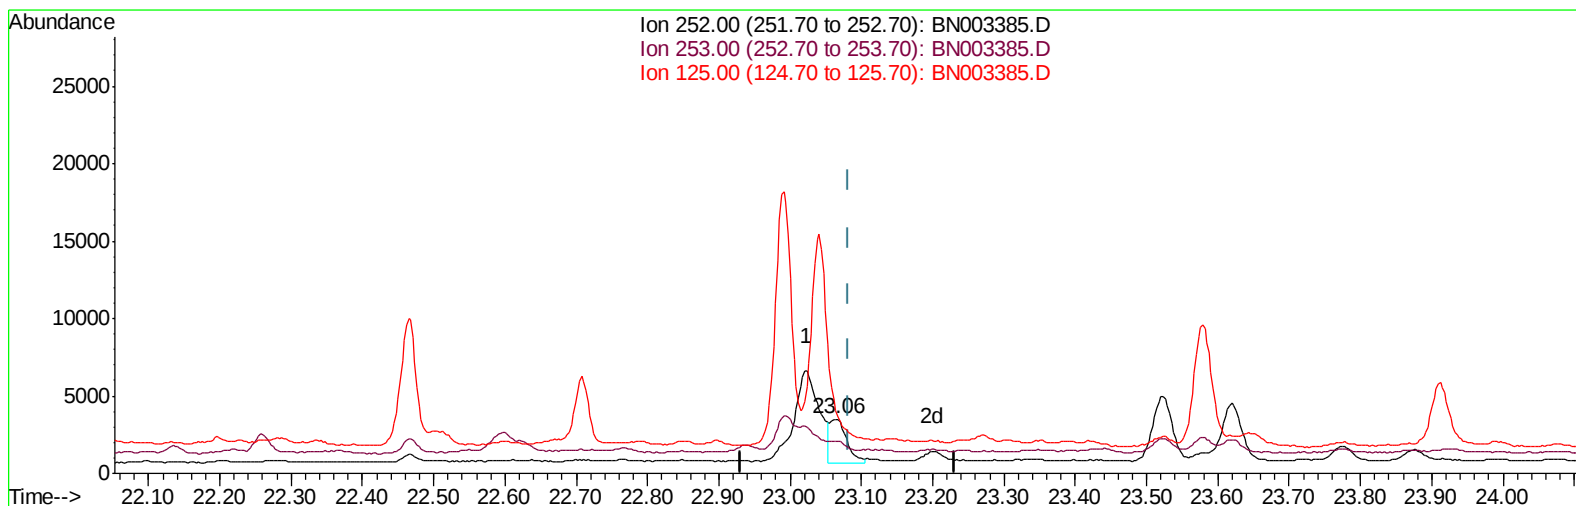

TIC: BN003385.D

(22) Benzo(k)fluoranthene

23.064min (-0.018) 0.02ng/ul m

response 4634

Ion	Exp%	Act%
252.00	100	100
253.00	22.80	59.87#
125.00	10.80	116.41#
0.00	0.00	0.00