
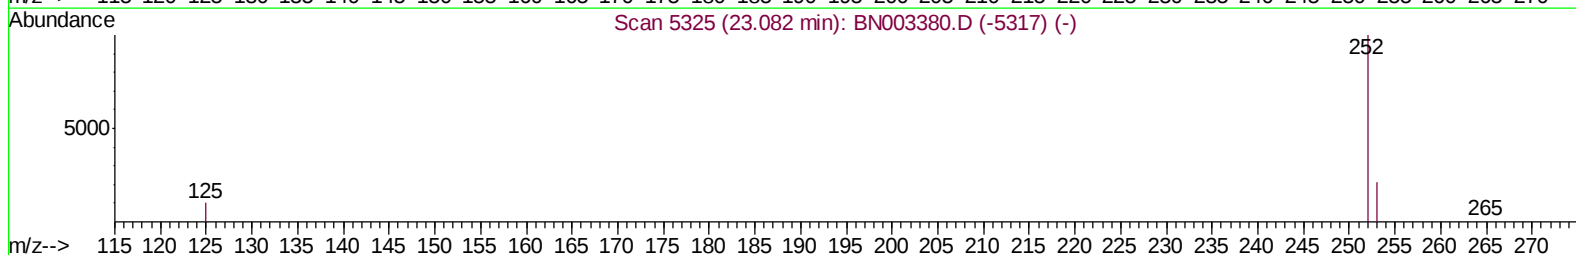
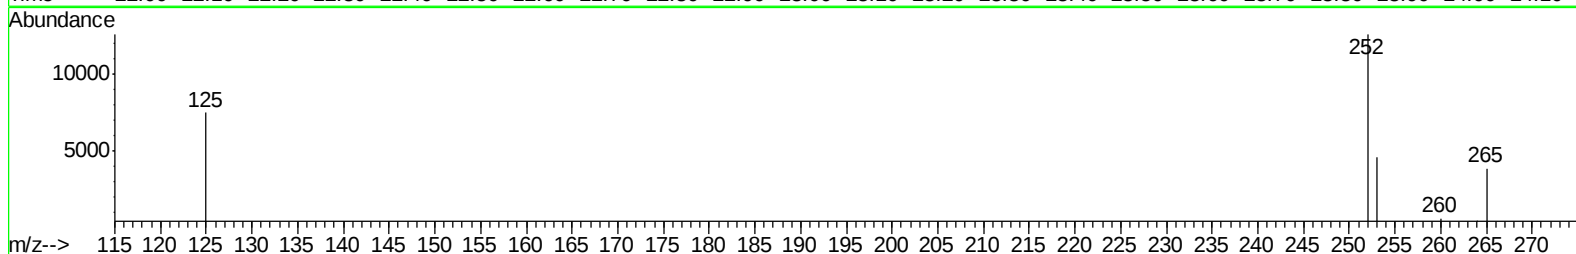


Data File : BN003386.D
Acq On : 01 Nov 2018 19:35
Operator : MJ/SJ
Sample : J5657-18MSD
Misc :
ALS Vial : 17 Sample Multiplier: 1

Quant Time: Nov 02 04:52:14 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 02 04:49:17 2018
Response via : Initial Calibration

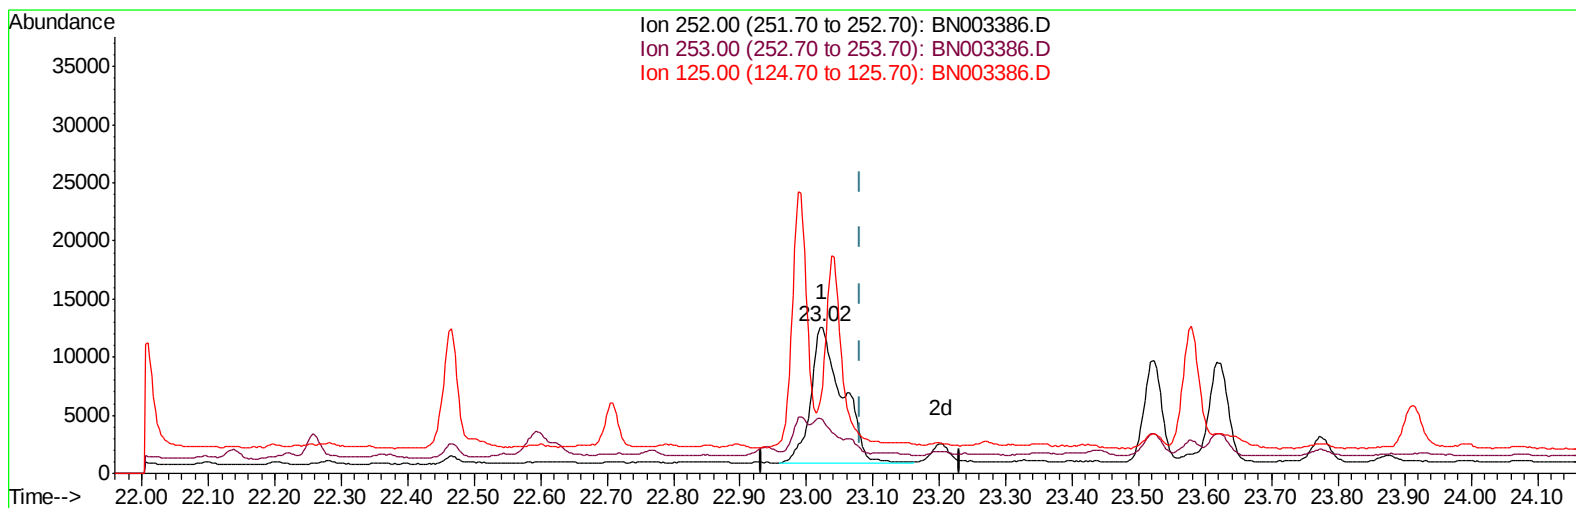

TIC: BN003386.D

(22) Benzo(k)fluoranthene
23.023min (-0.059) 0.18ng/ul
response 38261

Ion	Exp%	Act%
252.00	100	100
253.00	22.80	36.84#
125.00	10.80	59.61#
0.00	0.00	0.00