
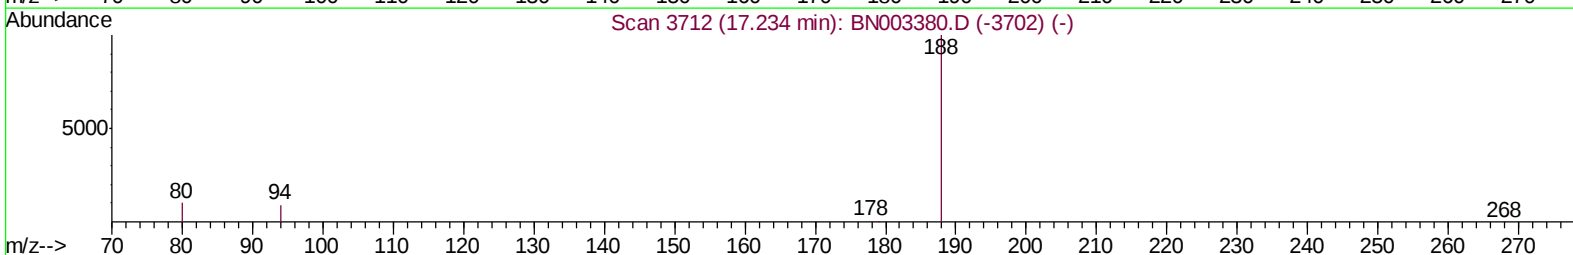
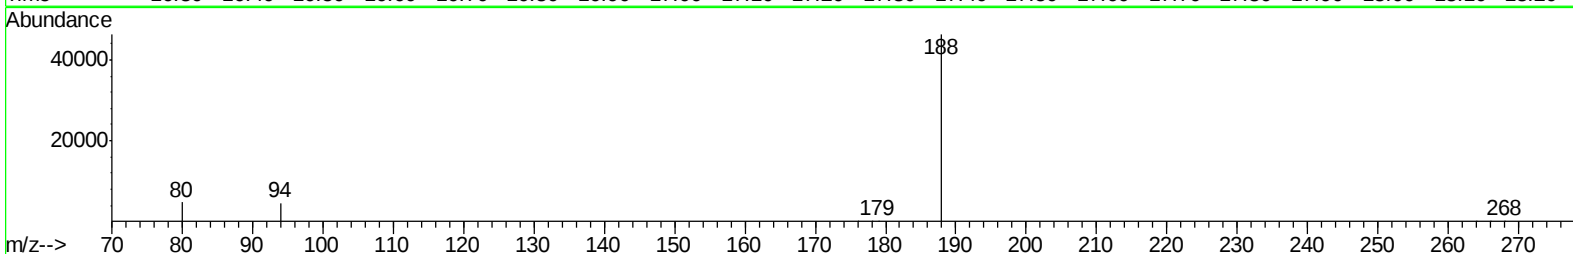


Data File : BN003387.D
Acq On : 01 Nov 2018 20:10
Operator : MJ/SJ
Sample : J5635-27
Misc :
ALS Vial : 18 Sample Multiplier: 1

Quant Time: Nov 02 04:52:25 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 02 04:49:17 2018
Response via : Initial Calibration

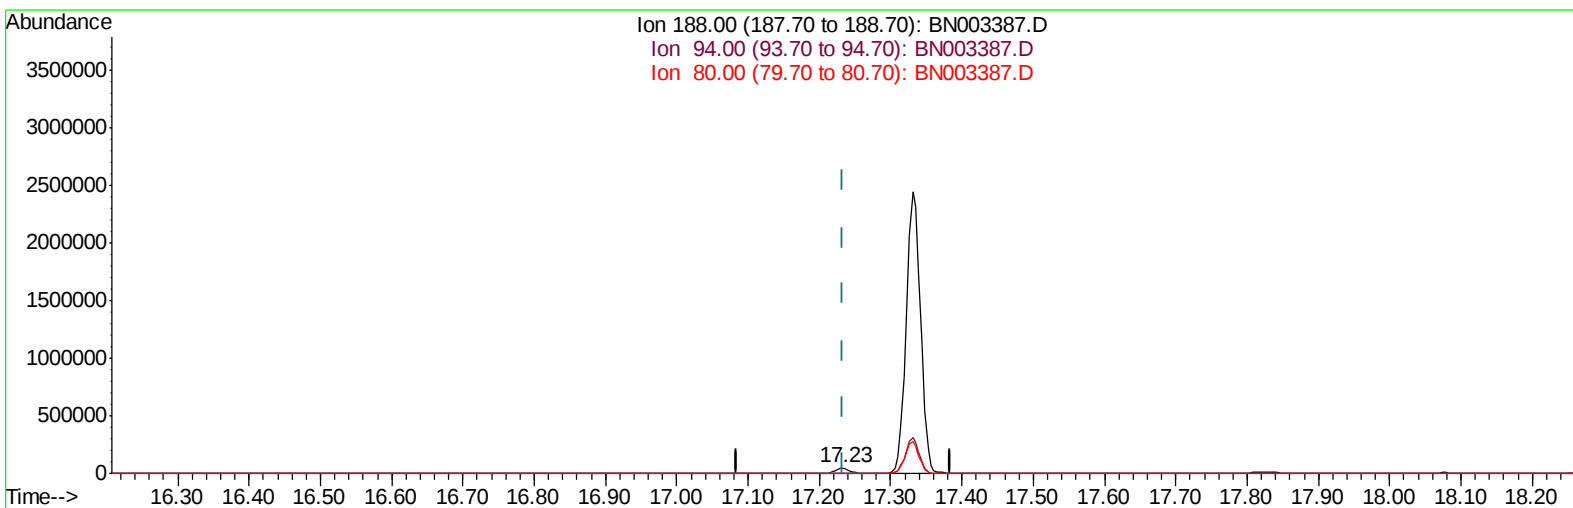

TIC: BN003387.D

(10) Phenanthrene-d10 (I)

17.234min (-0.000) 0.40ng/ul m

response 64215

Ion	Exp%	Act%
188.00	100	100
94.00	9.20	9.76
80.00	10.10	10.35
0.00	0.00	0.00