
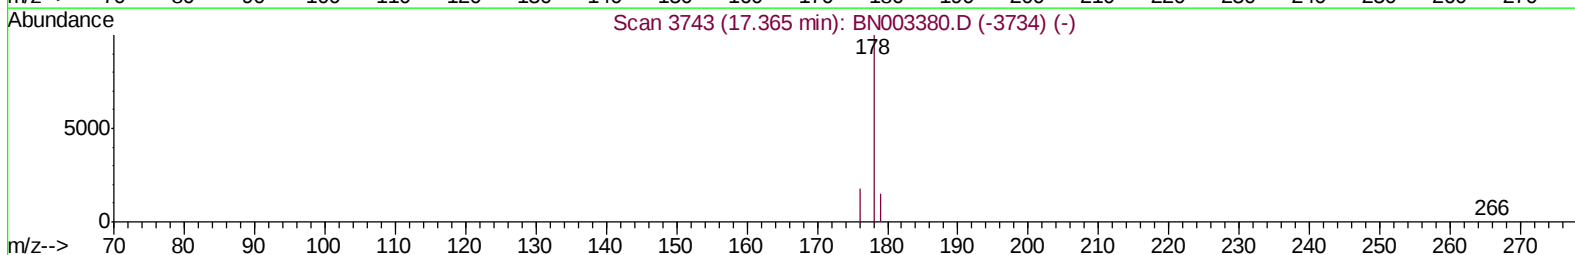
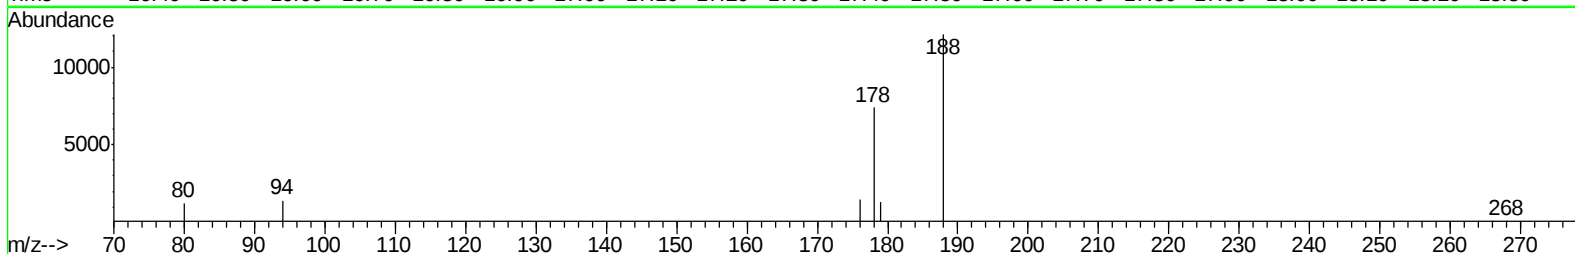


Data File : BN003387.D  
Acq On : 01 Nov 2018 20:10  
Operator : MJ/SJ  
Sample : J5635-27  
Misc :  
ALS Vial : 18 Sample Multiplier: 1

Quant Time: Nov 02 05:11:07 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\SOM-EPA-SIM-BN110118.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Nov 02 04:49:17 2018  
Response via : Initial Calibration

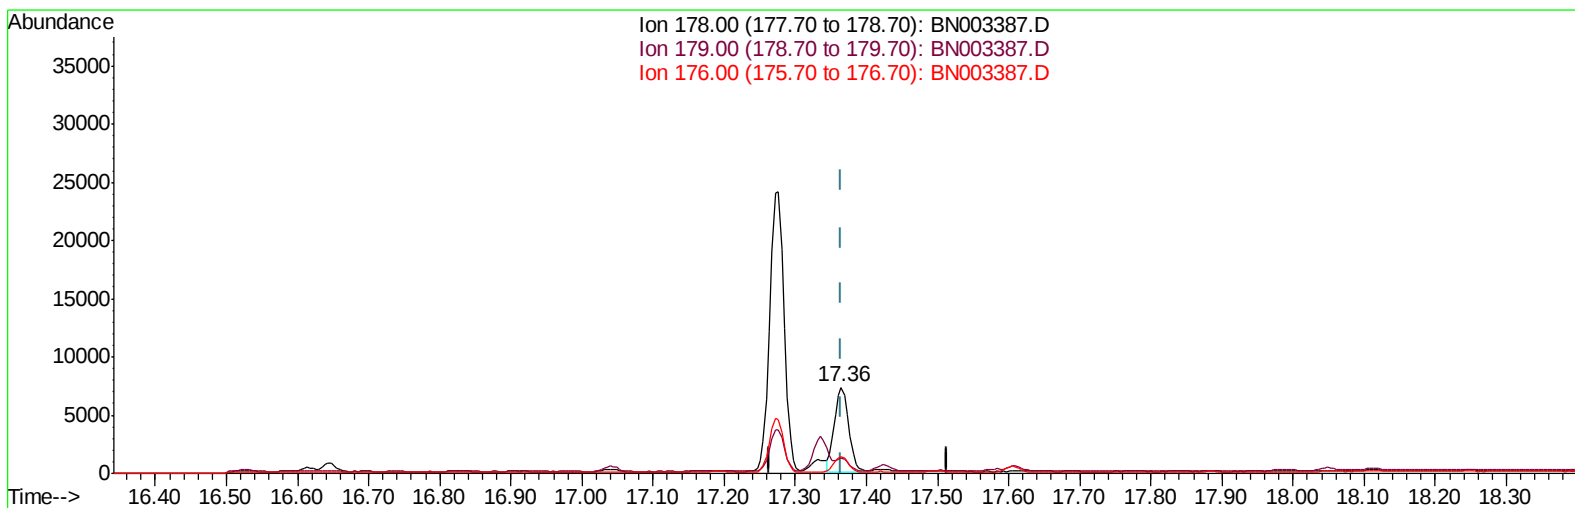

TIC: BN003387.D

(13) Anthracene

17.365min (-0.000) 0.06ng/ul m

response 10384

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 178.00 | 100   | 100   |
| 179.00 | 15.20 | 17.85 |
| 176.00 | 18.40 | 19.25 |
| 0.00   | 0.00  | 0.00  |