
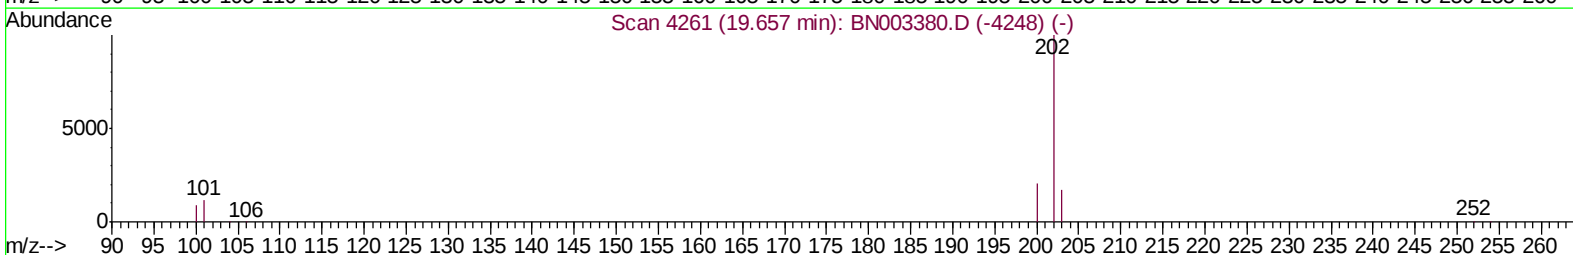
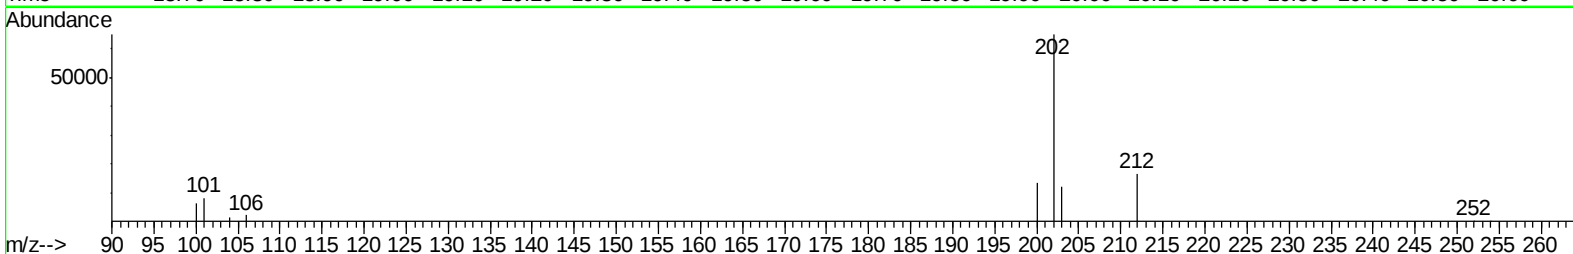


Data File : BN003387.D
Acq On : 01 Nov 2018 20:10
Operator : MJ/SJ
Sample : J5635-27
Misc :
ALS Vial : 18 Sample Multiplier: 1

Quant Time: Nov 02 05:12:48 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 02 04:49:17 2018
Response via : Initial Calibration

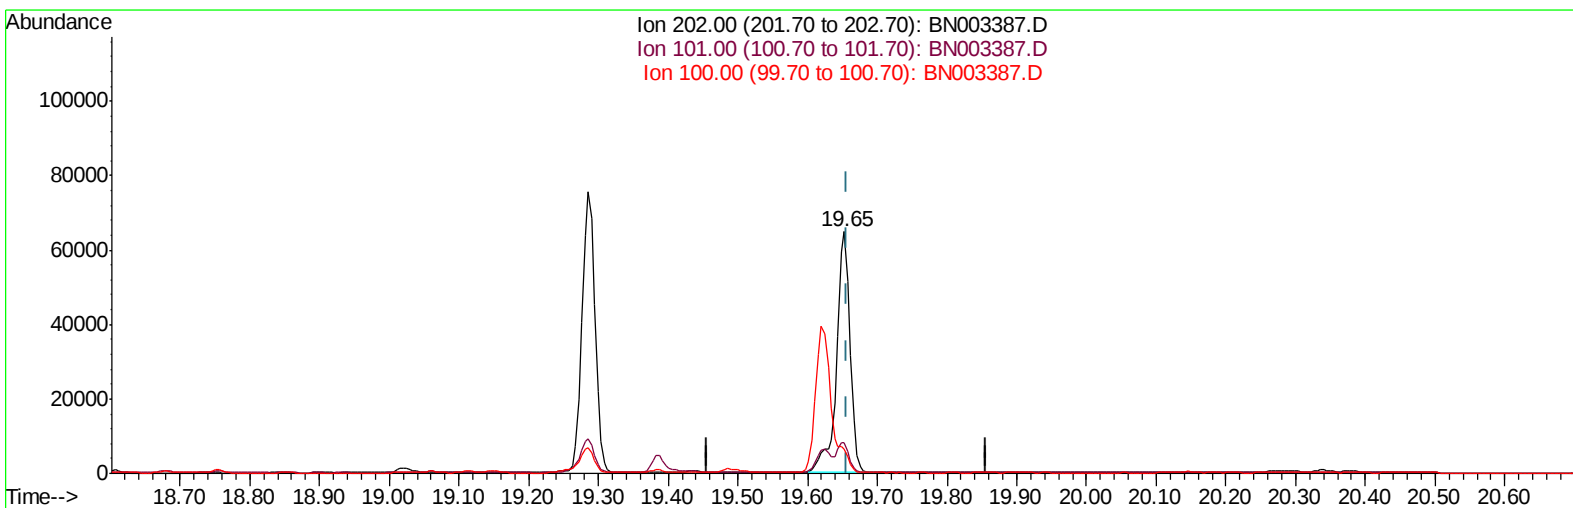

TIC: BN003387.D

(17) Pyrene

19.653min (-0.005) 0.39ng/ul

response 87335

Ion	Exp%	Act%
202.00	100	100
101.00	11.90	12.68
100.00	9.40	10.03
0.00	0.00	0.00