
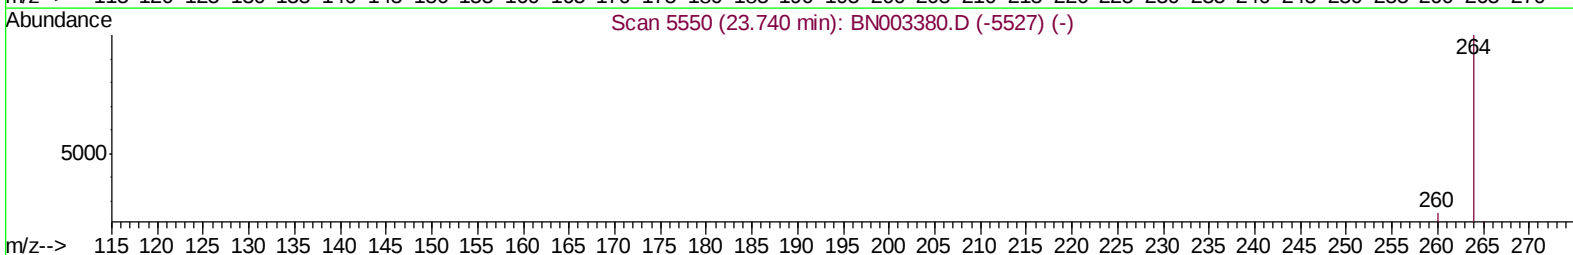
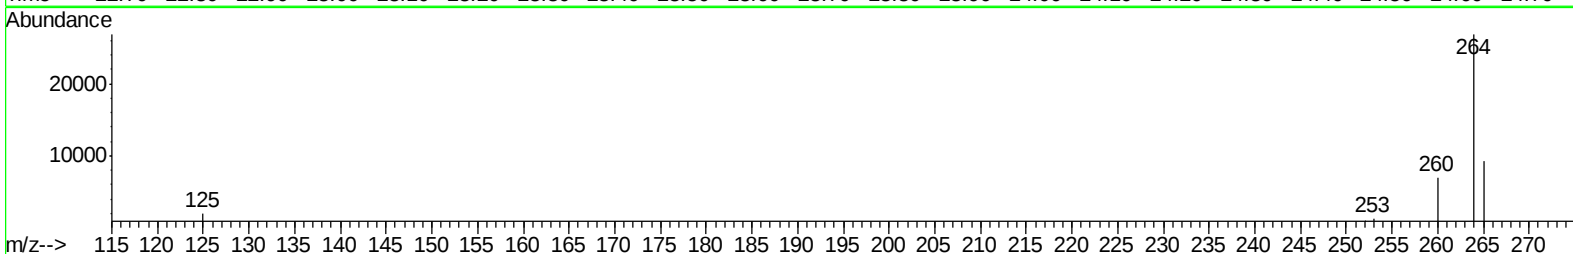


Data File : BN003387.D
Acq On : 01 Nov 2018 20:10
Operator : MJ/SJ
Sample : J5635-27
Misc :
ALS Vial : 18 Sample Multiplier: 1

Quant Time: Nov 02 05:12:48 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 02 04:49:17 2018
Response via : Initial Calibration

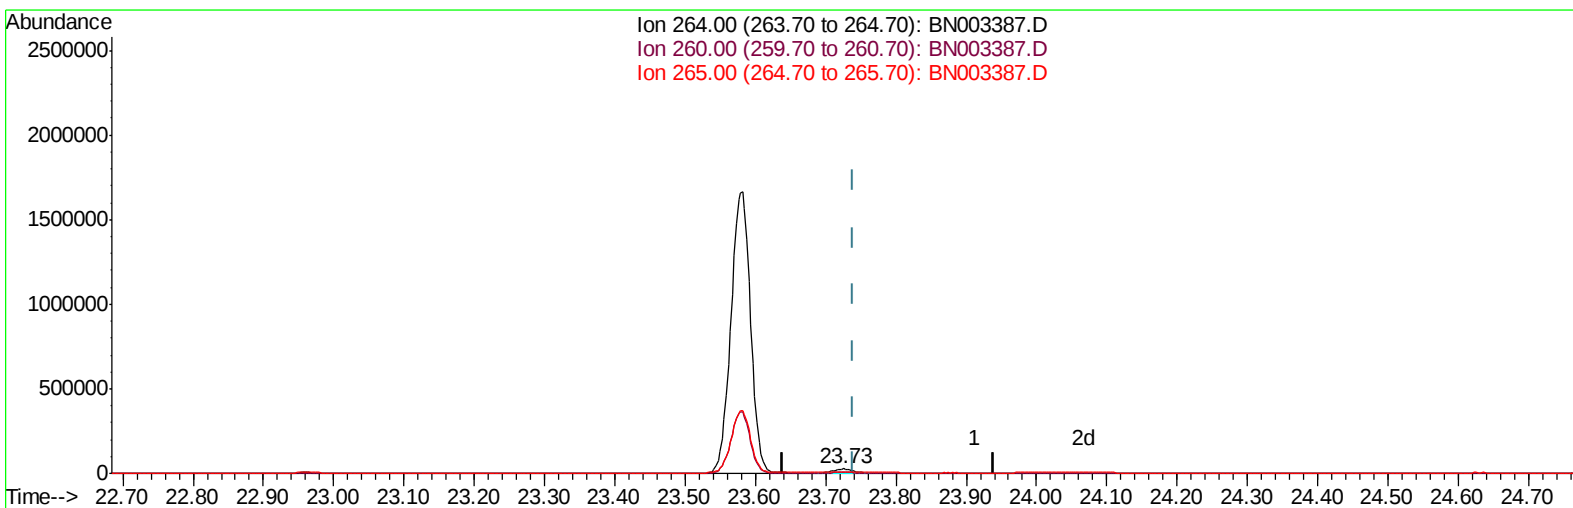

TIC: BN003387.D

(20) Perylene-d12 (I)

23.725min (-0.015) 0.40ng/ul m

response 49310

Ion	Exp%	Act%
264.00	100	100
260.00	25.60	26.13
265.00	33.70	34.70
0.00	0.00	0.00