
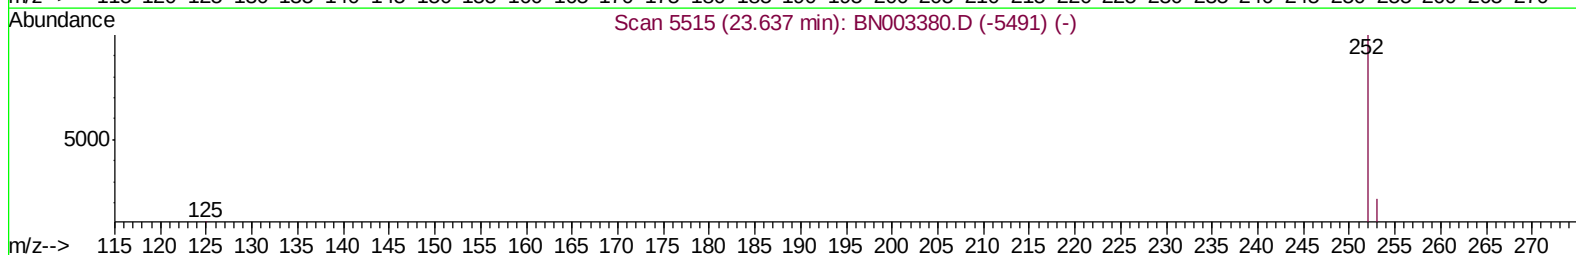
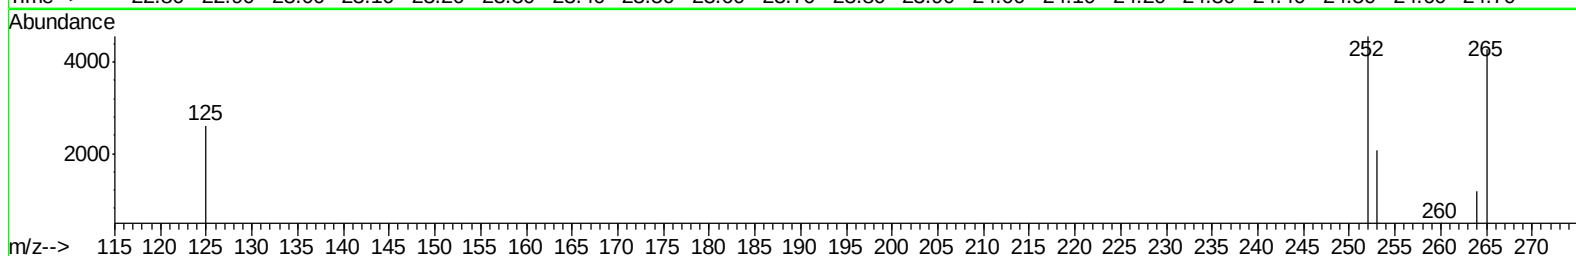


Data File : BN003387.D
Acq On : 01 Nov 2018 20:10
Operator : MJ/SJ
Sample : J5635-27
Misc :
ALS Vial : 18 Sample Multiplier: 1

Quant Time: Nov 02 05:13:59 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 02 04:49:17 2018
Response via : Initial Calibration

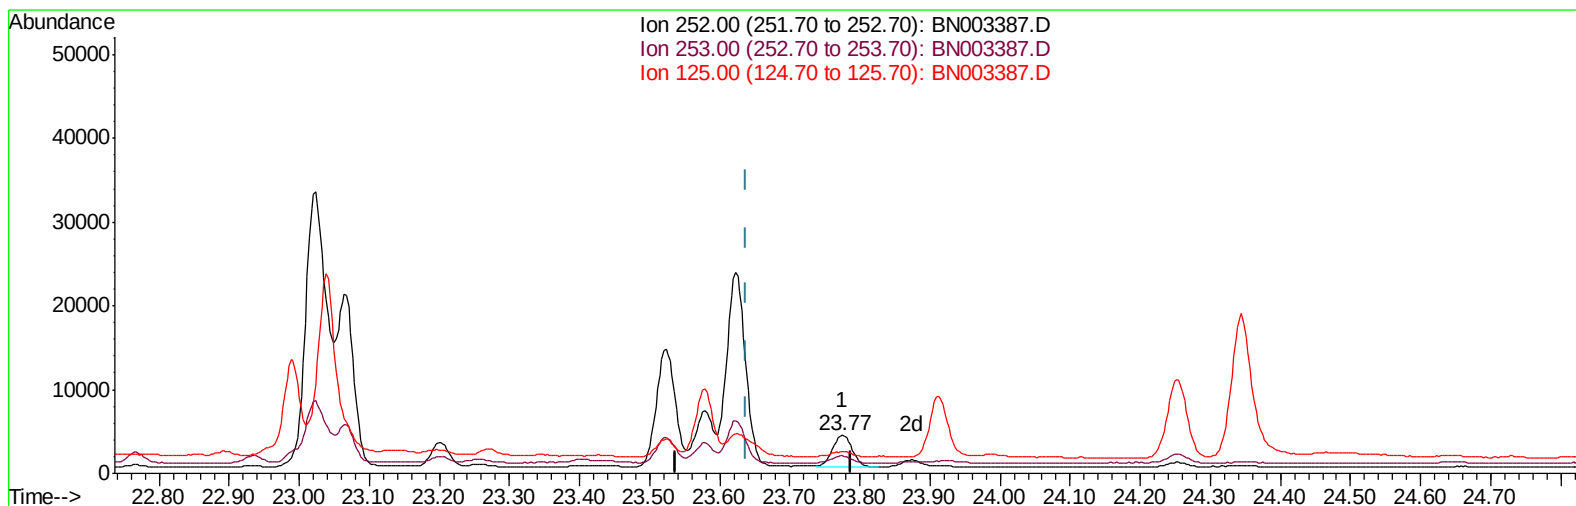

TIC: BN003387.D

(23) Benzo(a)pyrene (C)
23.775min (+0.137) 0.04ng/ul
response 7300

Ion	Exp%	Act%
252.00	100	100
253.00	23.10	45.63#
125.00	12.40	57.29#
0.00	0.00	0.00