
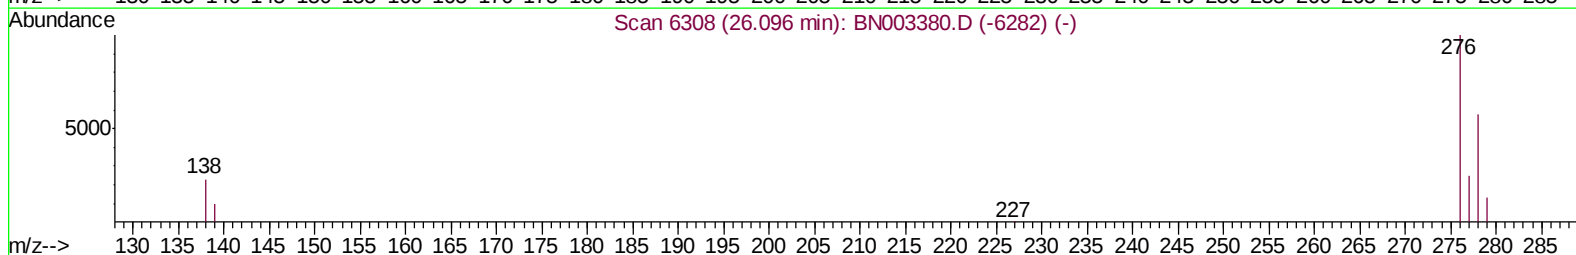
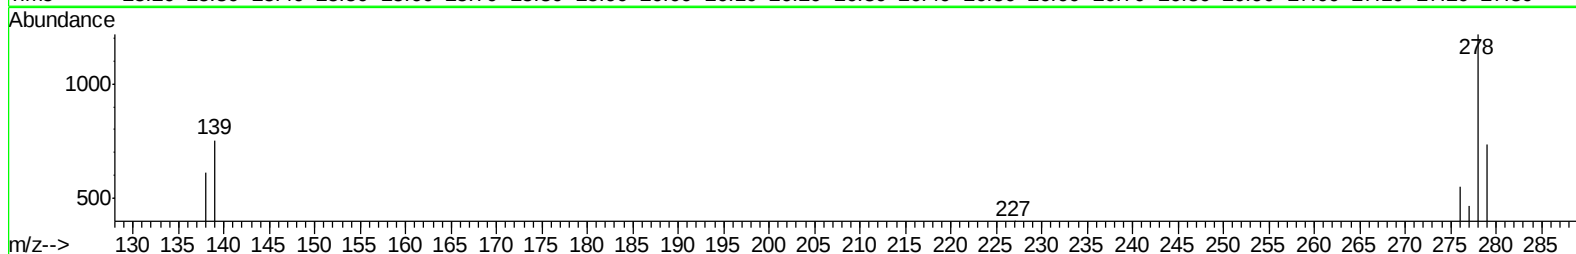


Data File : BN003387.D
Acq On : 01 Nov 2018 20:10
Operator : MJ/SJ
Sample : J5635-27
Misc :
ALS Vial : 18 Sample Multiplier: 1

Quant Time: Nov 02 05:13:59 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 02 04:49:17 2018
Response via : Initial Calibration

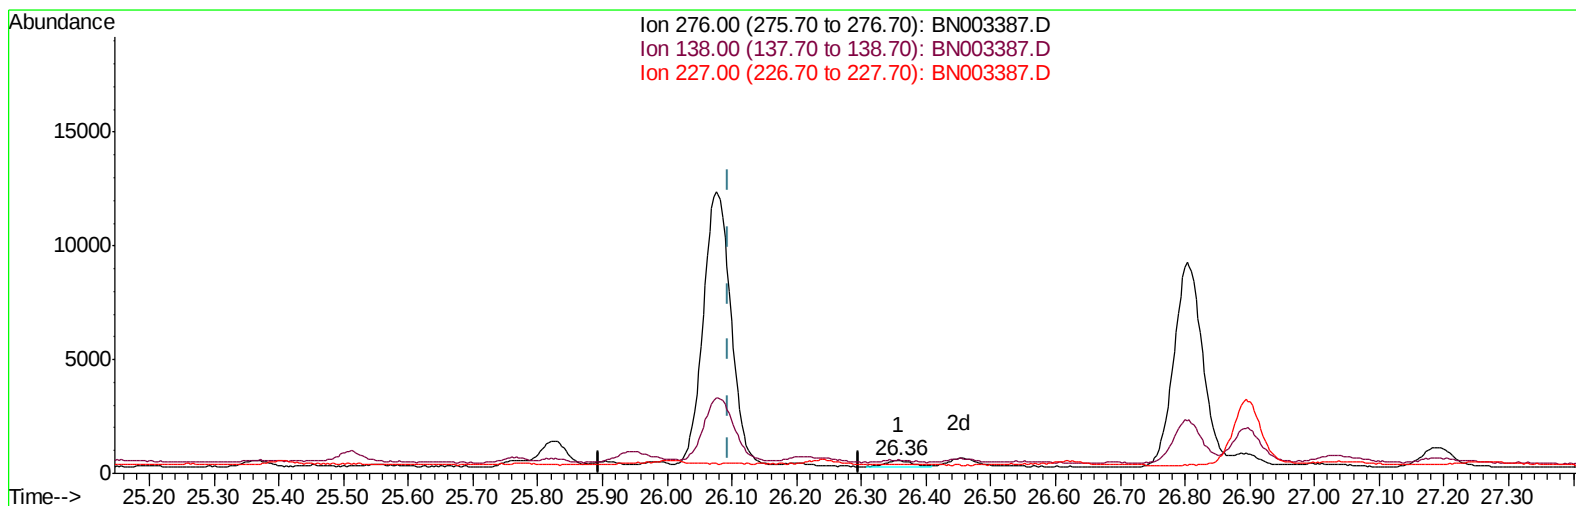

TIC: BN003387.D

(24) Indeno(1,2,3-cd)pyrene

26.357min (+0.262) 0.00ng/ul

response 791

Ion	Exp%	Act%
276.00	100	100
138.00	24.80	46.02#
227.00	0.20	18.71#
0.00	0.00	0.00