
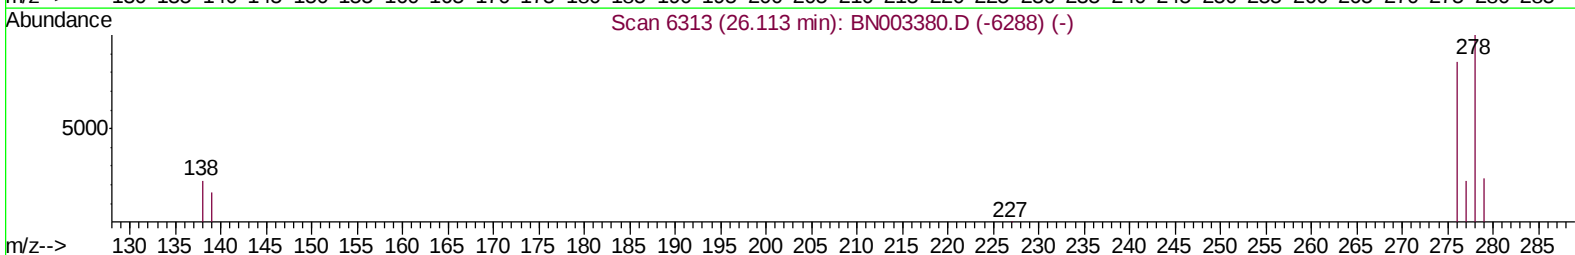
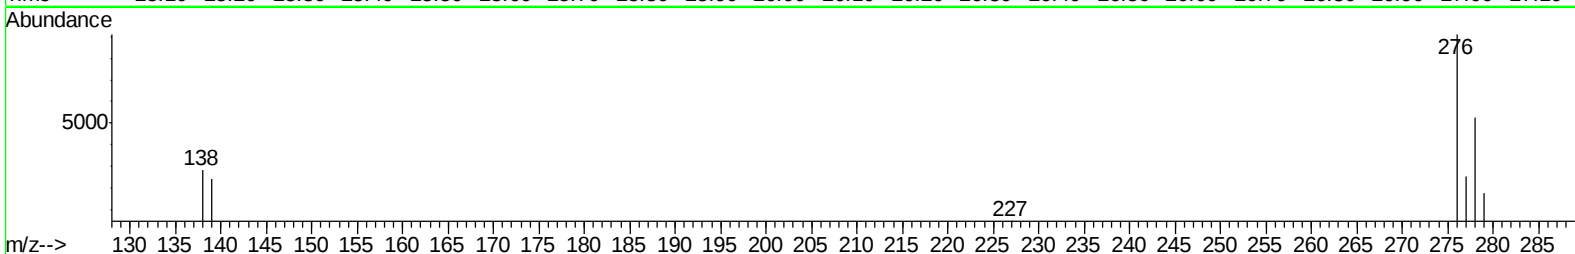


Data File : BN003387.D
Acq On : 01 Nov 2018 20:10
Operator : MJ/SJ
Sample : J5635-27
Misc :
ALS Vial : 18 Sample Multiplier: 1

Quant Time: Nov 02 05:13:59 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 02 04:49:17 2018
Response via : Initial Calibration

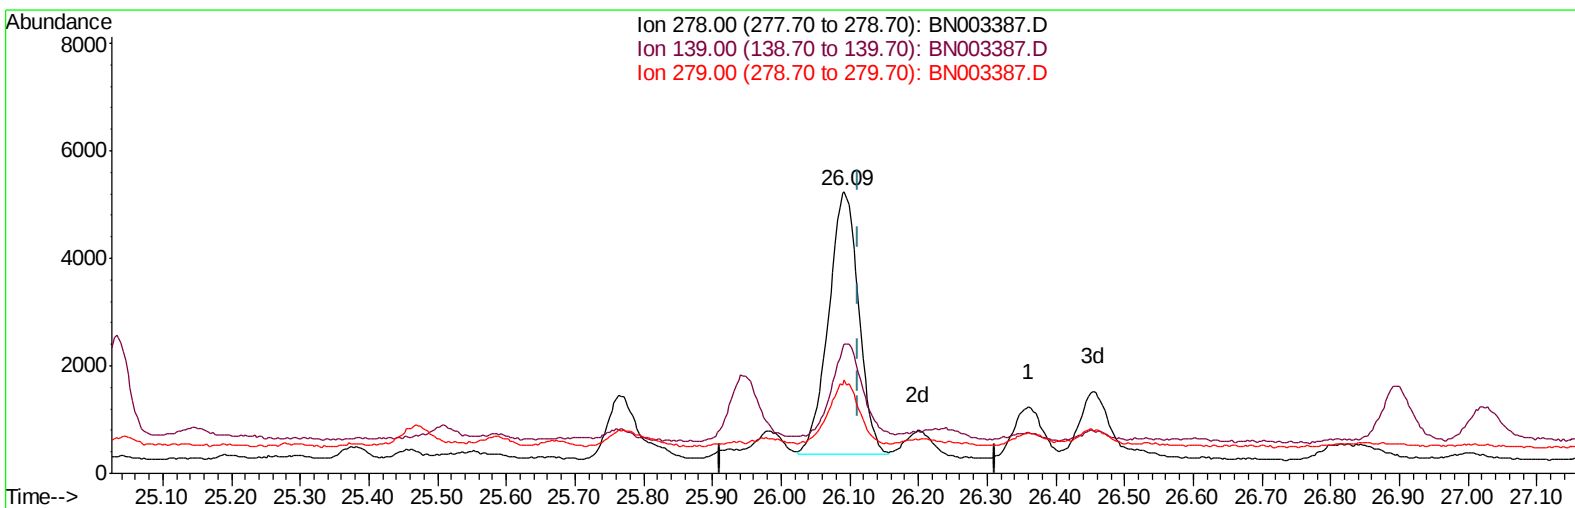

TIC: BN003387.D

(25) Dibenzo(a,h)anthracene

26.092min (-0.020) 0.10ng/ul m

response 14881

Ion	Exp%	Act%
278.00	100	100
139.00	16.40	45.81#
279.00	24.40	33.21#
0.00	0.00	0.00