
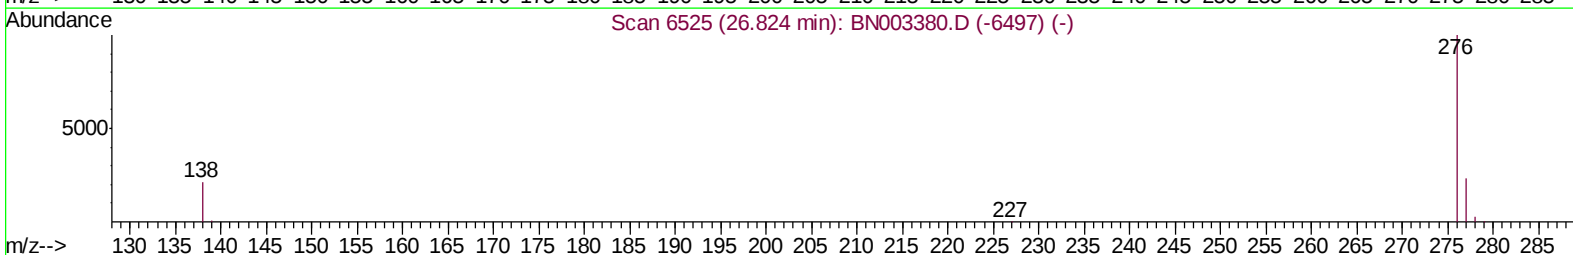
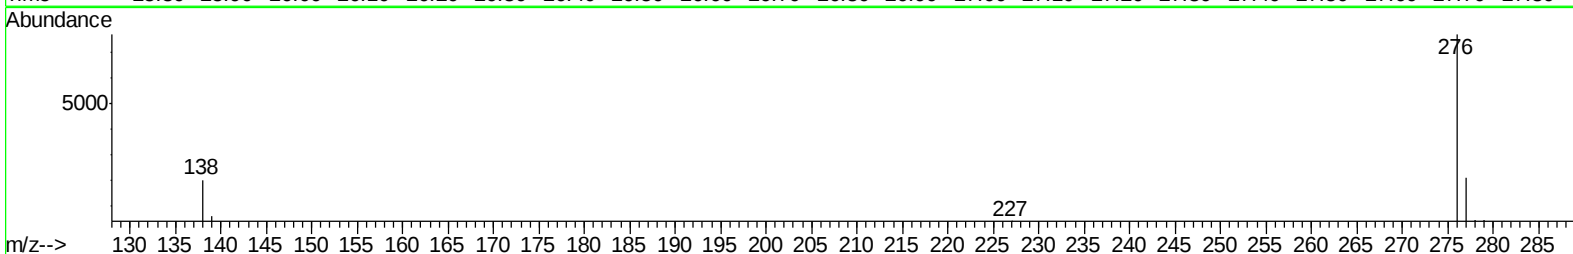


Data File : BN003389.D
Acq On : 01 Nov 2018 21:20
Operator : MJ/SJ
Sample : J5635-29MSD
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Nov 02 04:52:48 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 02 04:49:17 2018
Response via : Initial Calibration

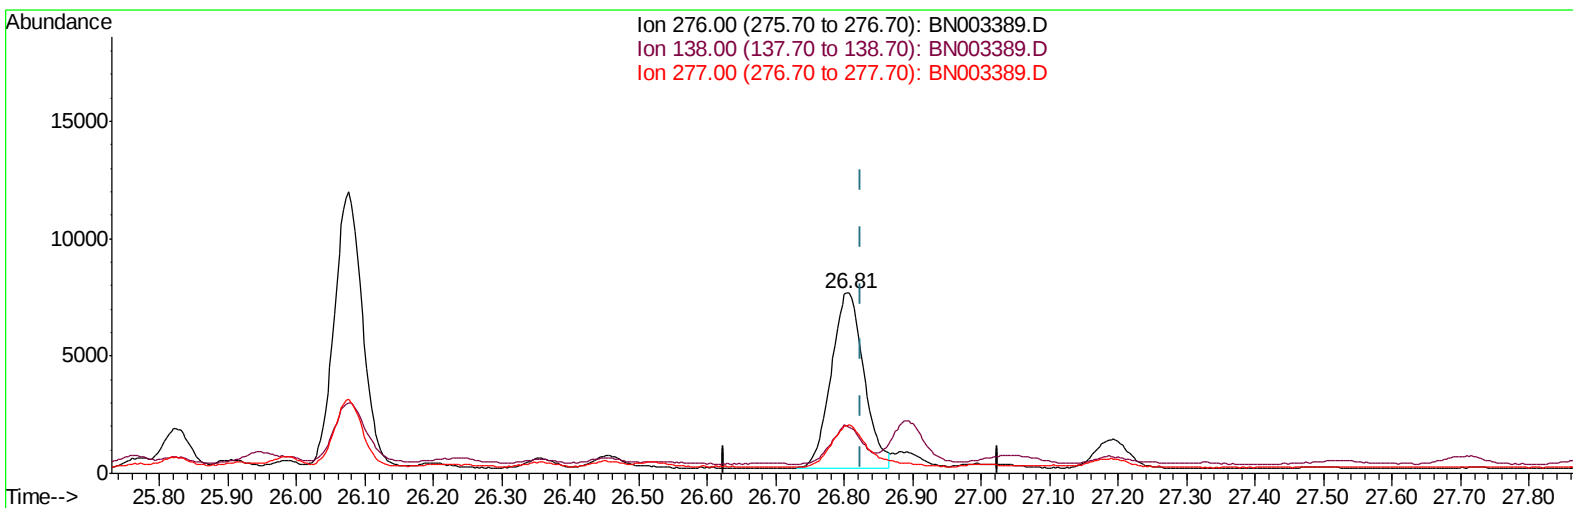

TIC: BN003389.D

(26) Benzo(g,h,i)perylene

26.807min (-0.017) 0.14ng/ul m

response 24989

Ion	Exp%	Act%
276.00	100	100
138.00	21.30	25.81#
277.00	24.00	26.92
0.00	0.00	0.00