
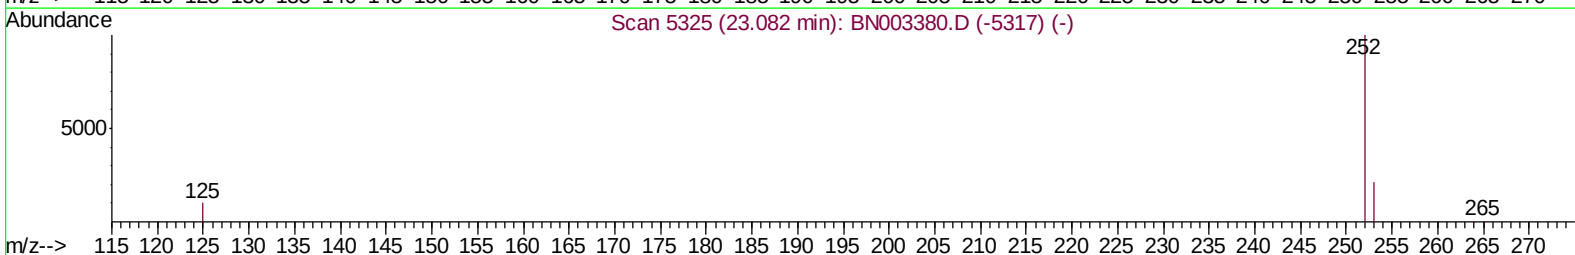
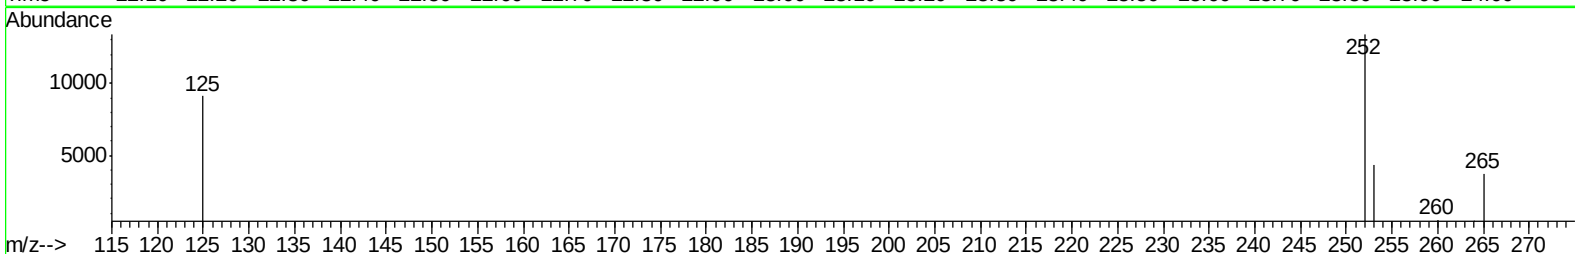


Data File : BN003390.D
Acq On : 01 Nov 2018 21:56
Operator : MJ/SJ
Sample : J5701-12
Misc :
ALS Vial : 21 Sample Multiplier: 1

Quant Time: Nov 02 05:23:36 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 02 04:49:17 2018
Response via : Initial Calibration

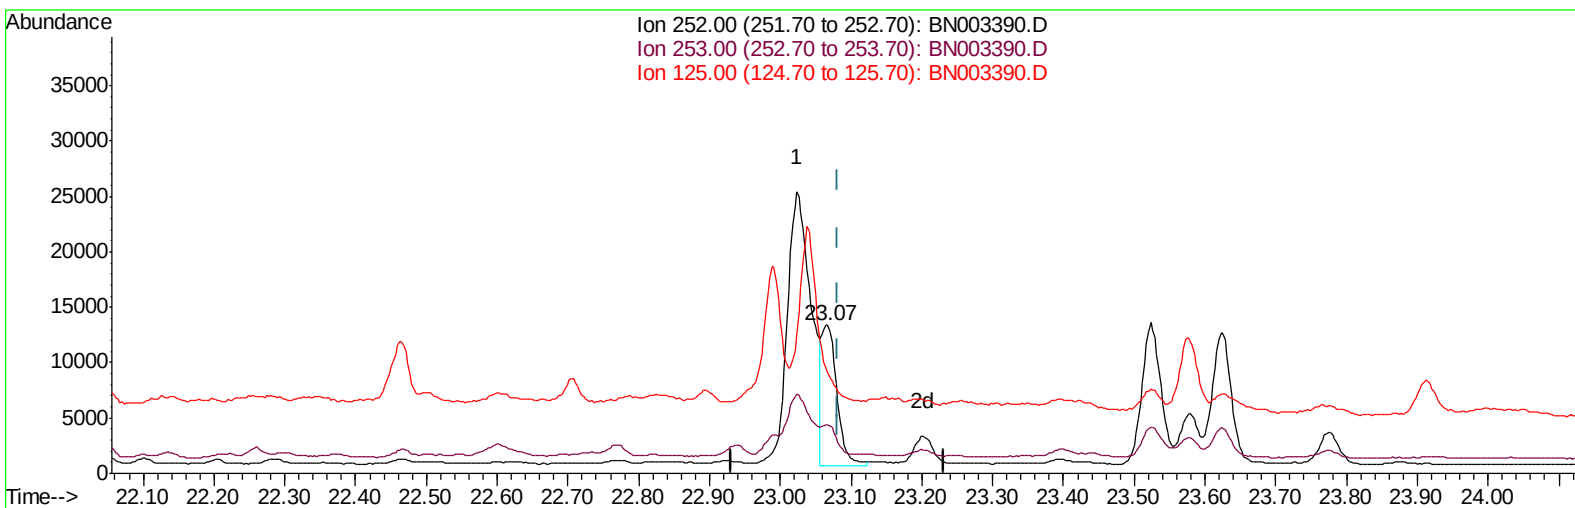

TIC: BN003390.D

(22) Benzo(k)fluoranthene

23.067min (-0.015) 0.09ng/ul m

response 19328

Ion	Exp%	Act%
252.00	100	100
253.00	22.80	32.74#
125.00	10.80	67.90#
0.00	0.00	0.00