
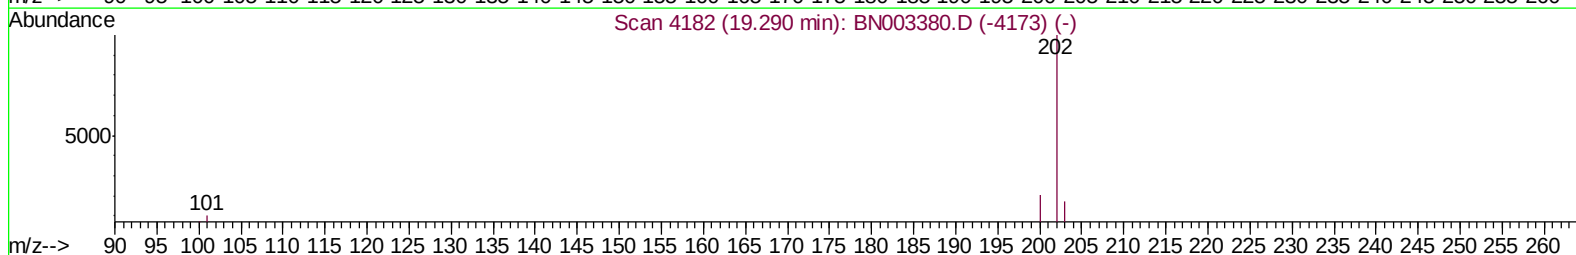
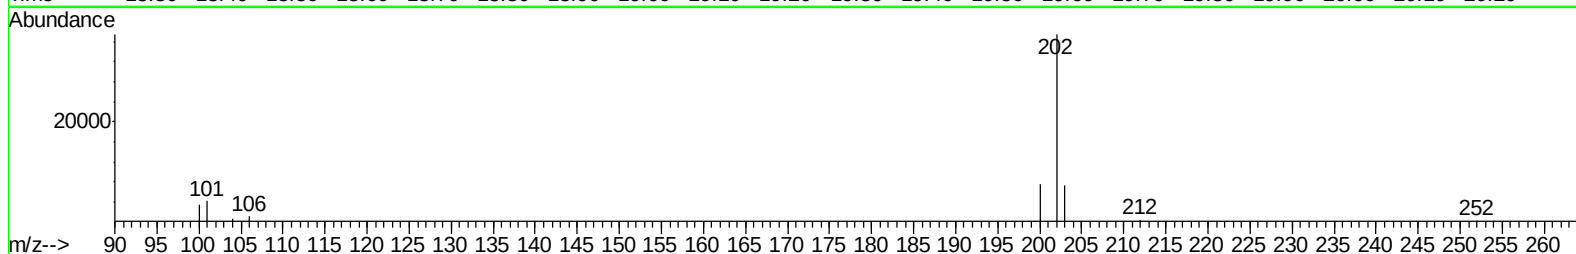


Data File : BN003392.D
Acq On : 01 Nov 2018 23:06
Operator : MJ/SJ
Sample : J5704-18
Misc :
ALS Vial : 23 Sample Multiplier: 1

Quant Time: Nov 02 05:40:28 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 02 04:49:17 2018
Response via : Initial Calibration

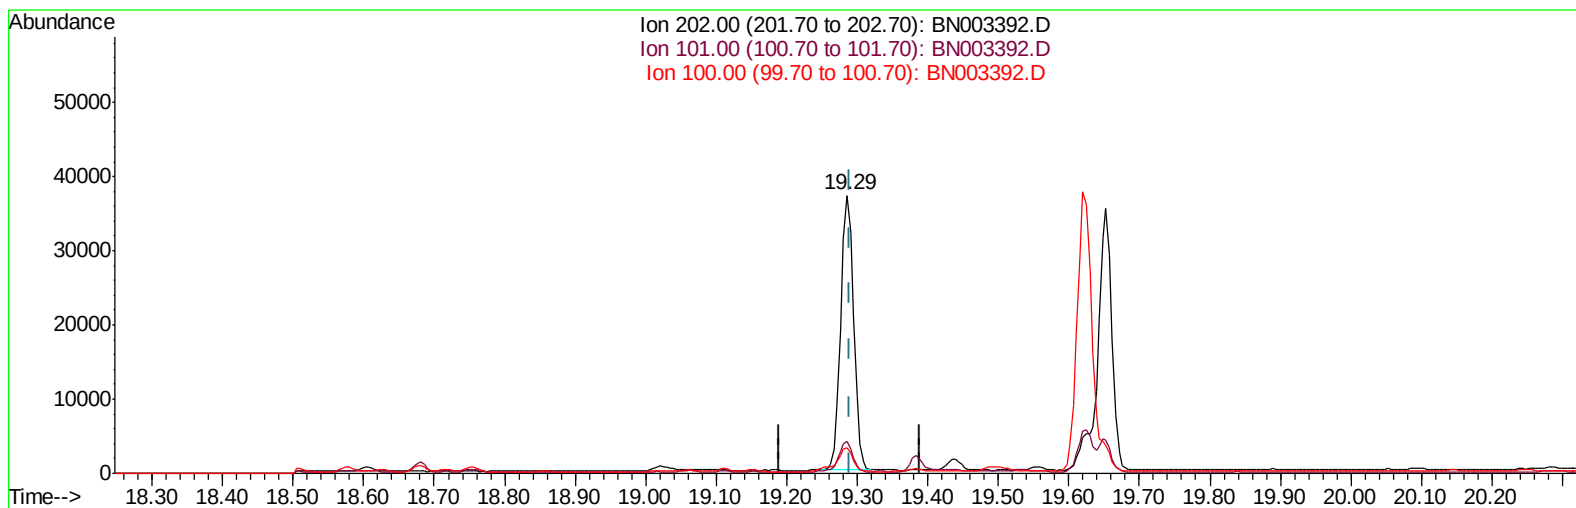

TIC: BN003392.D

(15) Fluoranthene (C)

19.285min (-0.005) 0.17ng/ul m

response 46403

Ion	Exp%	Act%
202.00	100	100
101.00	10.70	11.35
100.00	8.00	9.40
0.00	0.00	0.00