
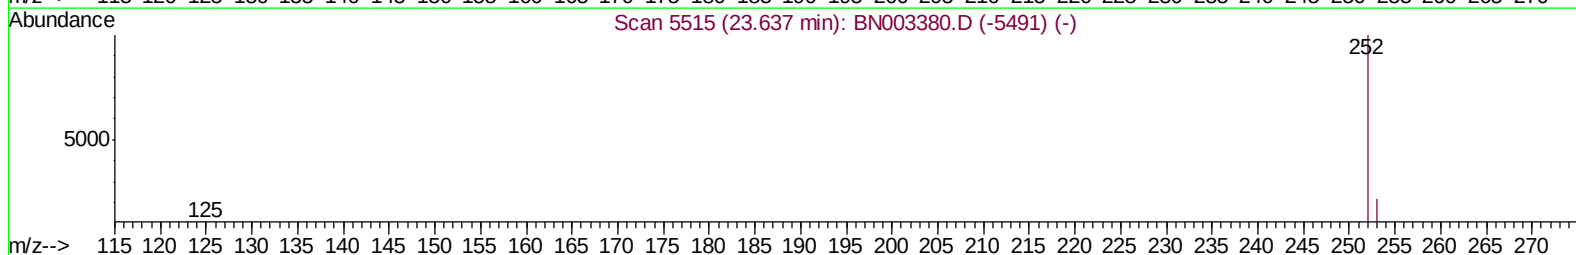
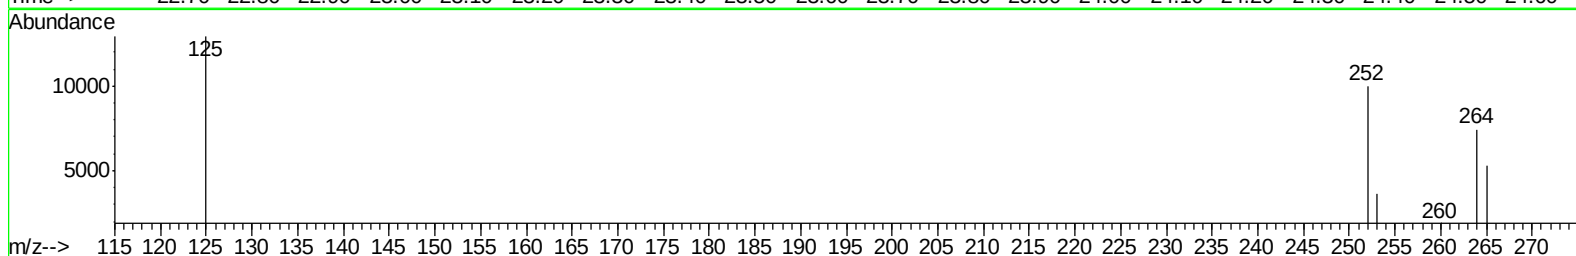


Data File : BN003392.D
Acq On : 01 Nov 2018 23:06
Operator : MJ/SJ
Sample : J5704-18
Misc :
ALS Vial : 23 Sample Multiplier: 1

Quant Time: Nov 02 05:43:14 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 02 04:49:17 2018
Response via : Initial Calibration

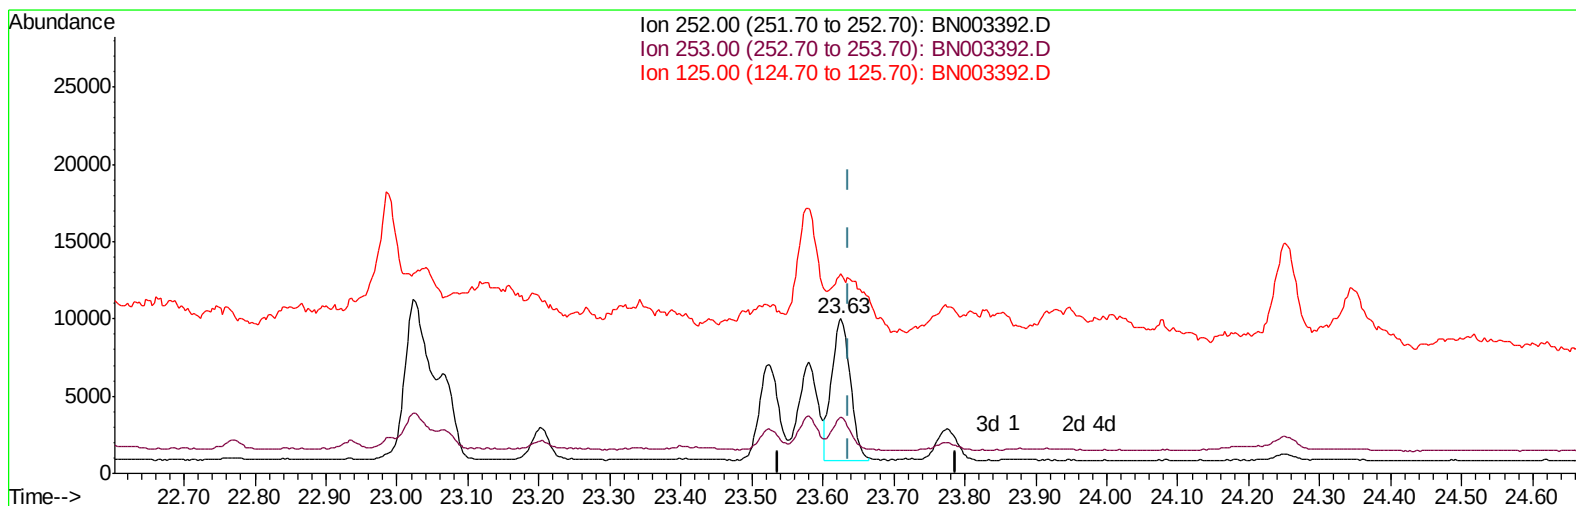

TIC: BN003392.D

(23) Benzo(a)pyrene (C)

23.626min (-0.012) 0.10ng/ul m

response 16597

Ion	Exp%	Act%
252.00	100	100
253.00	23.10	36.10#
125.00	12.40	129.15#
0.00	0.00	0.00