
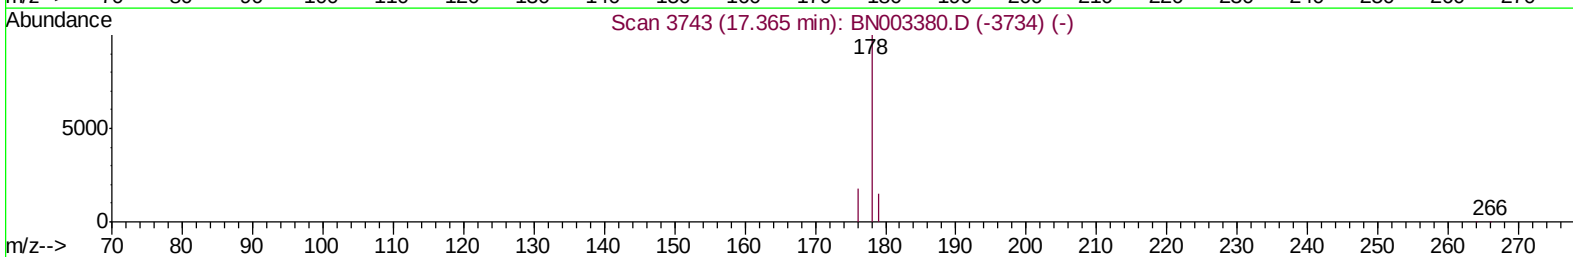
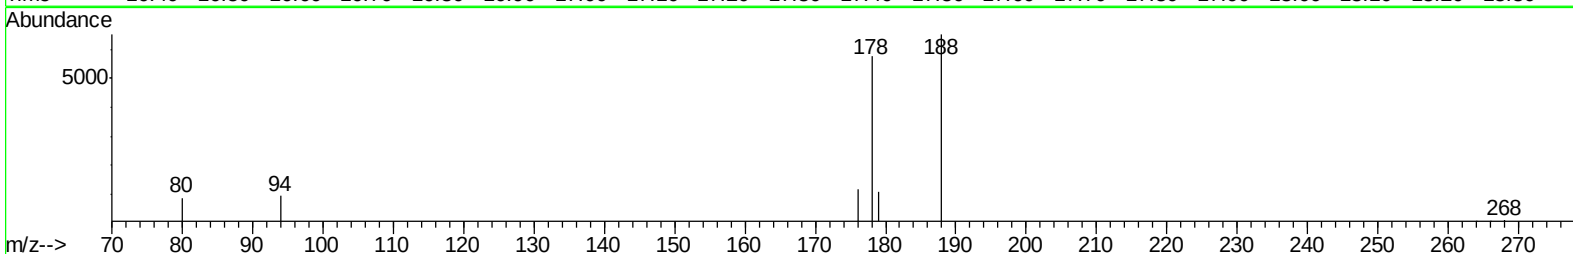


Data File : BN003393.D
Acq On : 01 Nov 2018 23:41
Operator : MJ/SJ
Sample : J5704-17
Misc :
ALS Vial : 24 Sample Multiplier: 1

Quant Time: Nov 02 05:56:10 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 02 04:49:17 2018
Response via : Initial Calibration

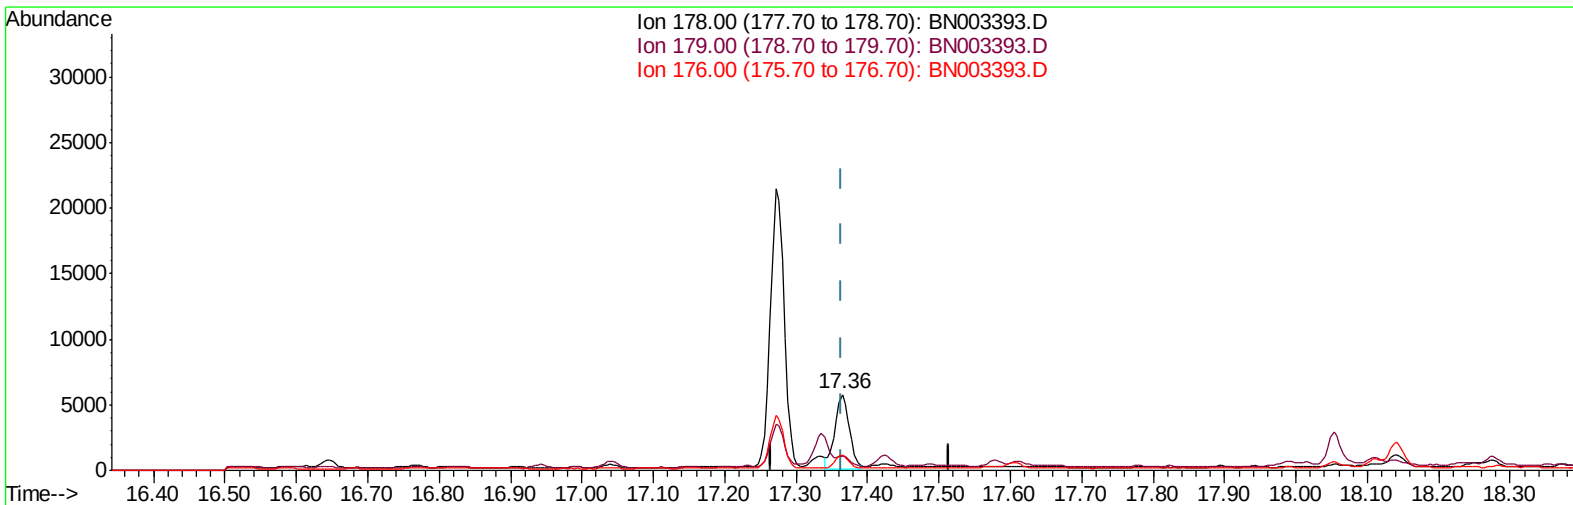

TIC: BN003393.D

(13) Anthracene

17.365min (-0.000) 0.05ng/ul m

response 8023

Ion	Exp%	Act%
178.00	100	100
179.00	15.20	19.10#
176.00	18.40	20.23
0.00	0.00	0.00