
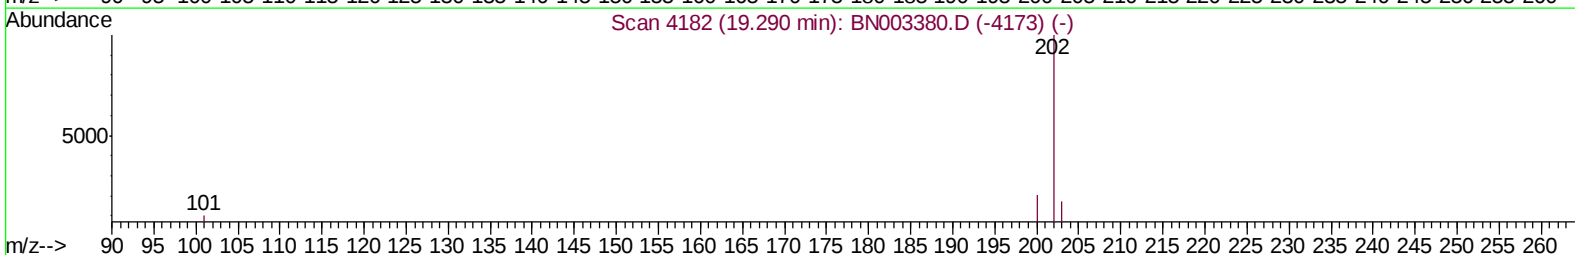
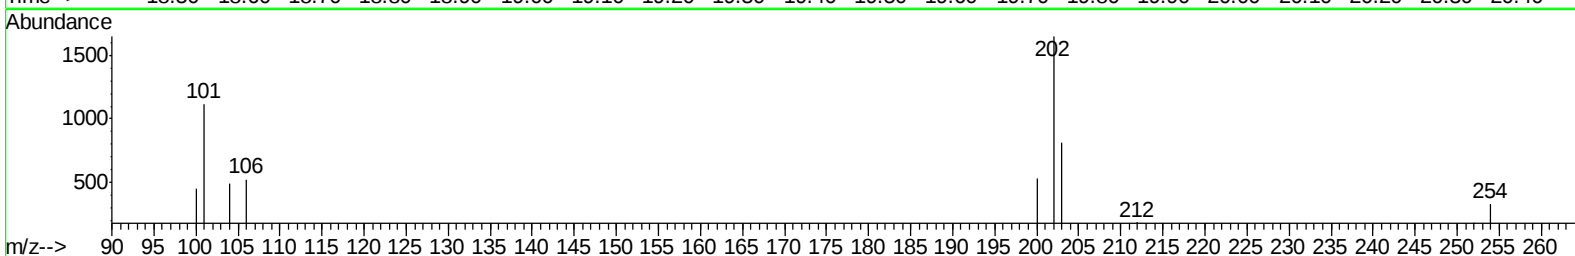


Data File : BN003393.D
Acq On : 01 Nov 2018 23:41
Operator : MJ/SJ
Sample : J5704-17
Misc :
ALS Vial : 24 Sample Multiplier: 1

Quant Time: Nov 02 05:56:10 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 02 04:49:17 2018
Response via : Initial Calibration

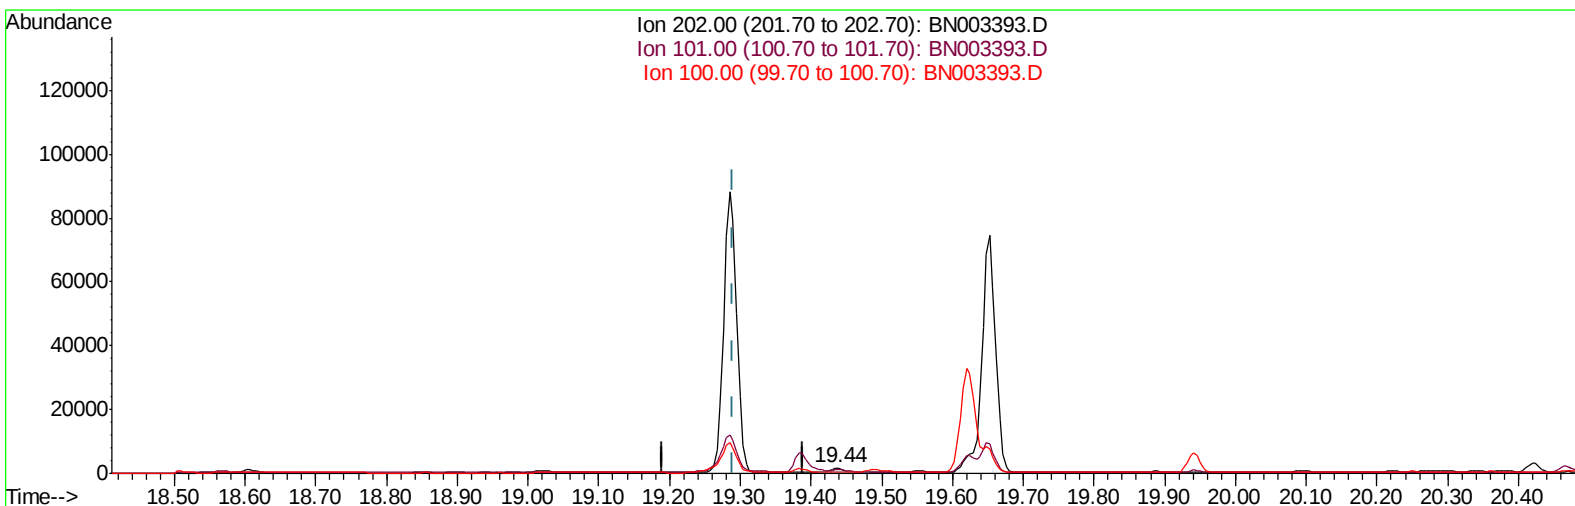

TIC: BN003393.D

(15) Fluoranthene (C)

19.439min (+0.149) 0.01ng/ul

response 1790

Ion	Exp%	Act%
202.00	100	100
101.00	10.70	67.78#
100.00	8.00	27.14
0.00	0.00	0.00