
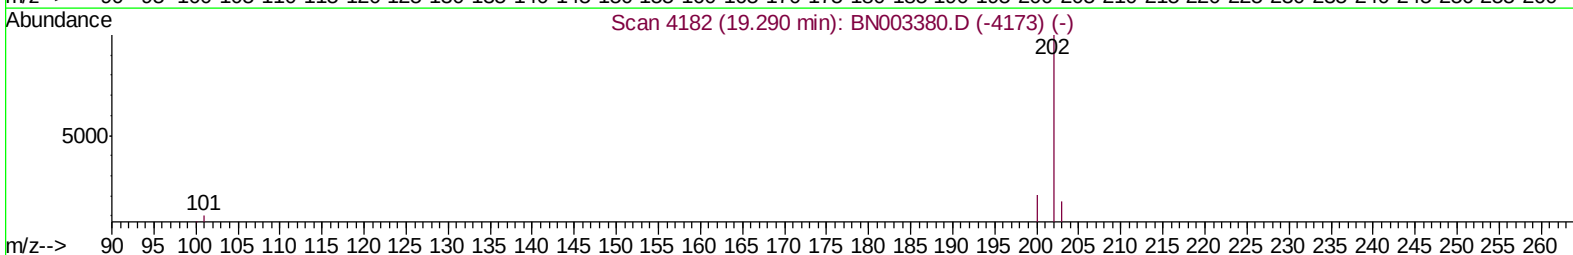
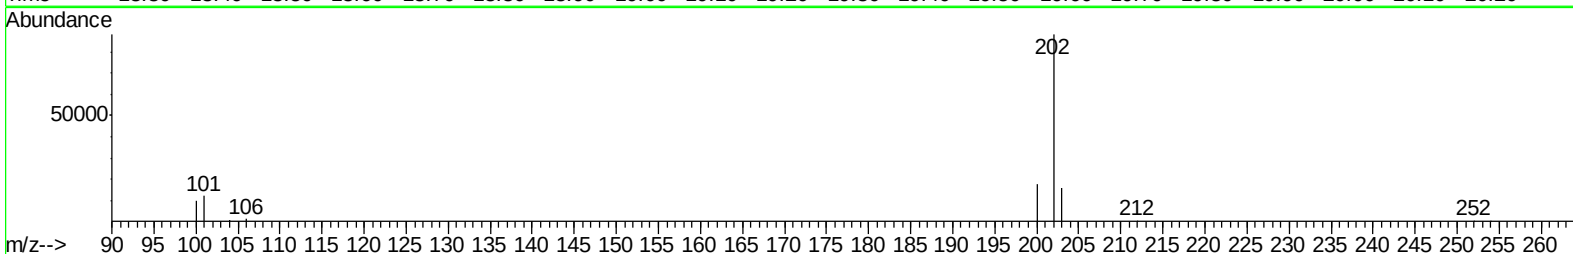


Data File : BN003393.D  
Acq On : 01 Nov 2018 23:41  
Operator : MJ/SJ  
Sample : J5704-17  
Misc :  
ALS Vial : 24 Sample Multiplier: 1

Quant Time: Nov 02 05:56:10 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\SOM-EPA-SIM-BN110118.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Nov 02 04:49:17 2018  
Response via : Initial Calibration

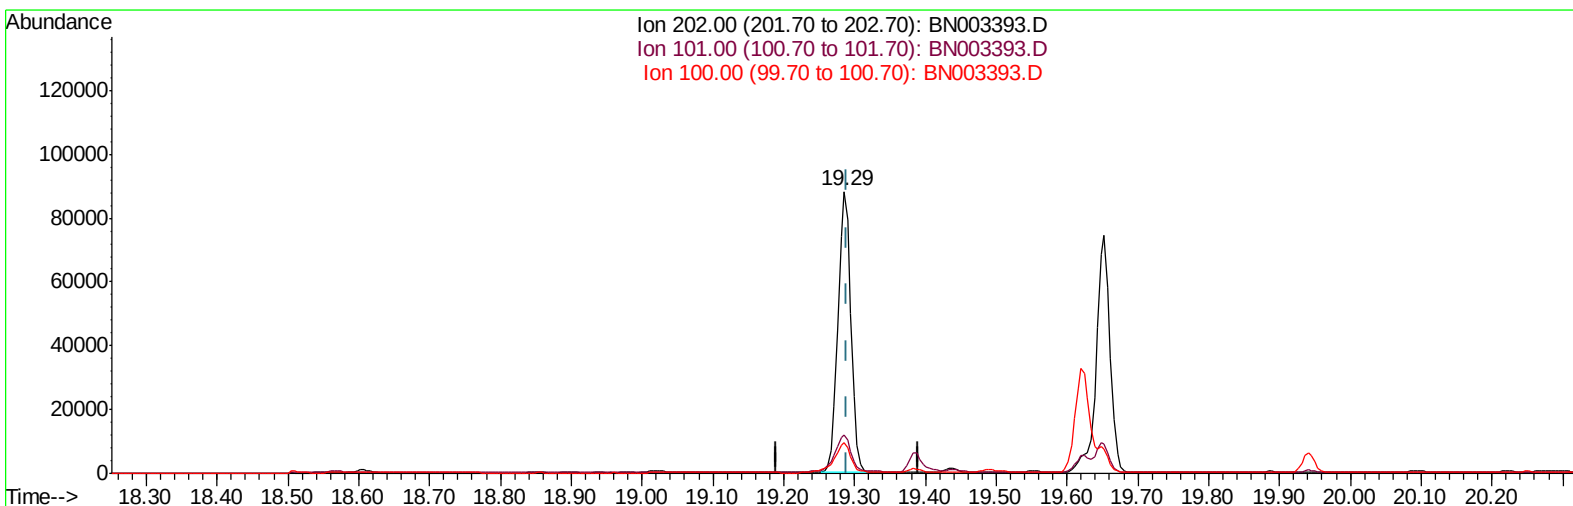

TIC: BN003393.D

(15) Fluoranthene (C)

19.285min (-0.005) 0.48ng/ul m

response 111612

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 202.00 | 100   | 100   |
| 101.00 | 10.70 | 13.60 |
| 100.00 | 8.00  | 11.08 |
| 0.00   | 0.00  | 0.00  |