
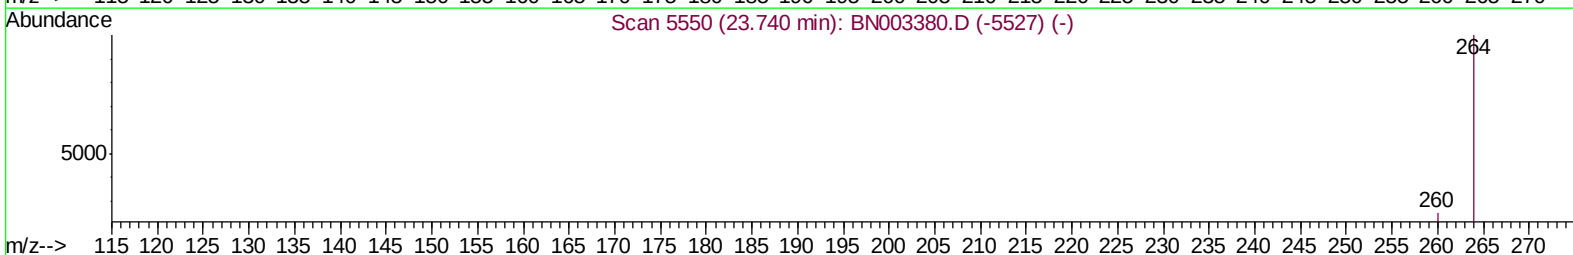
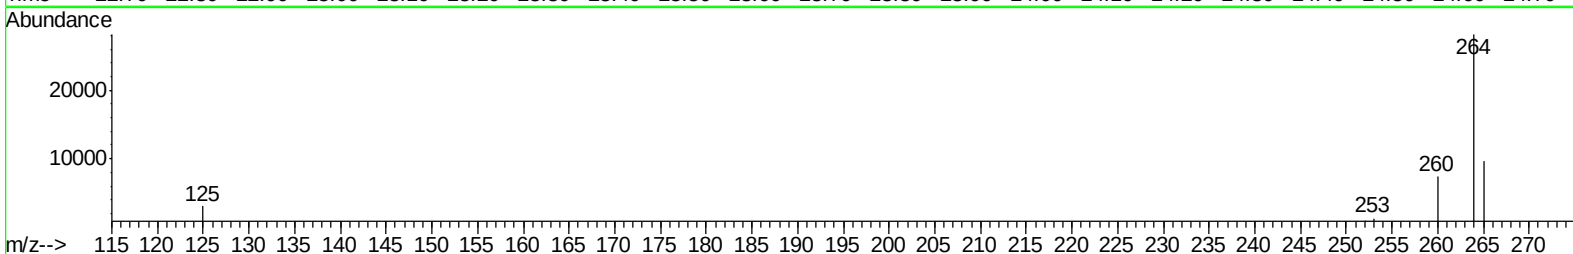


Data File : BN003393.D
Acq On : 01 Nov 2018 23:41
Operator : MJ/SJ
Sample : J5704-17
Misc :
ALS Vial : 24 Sample Multiplier: 1

Quant Time: Nov 02 05:57:20 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 02 04:49:17 2018
Response via : Initial Calibration

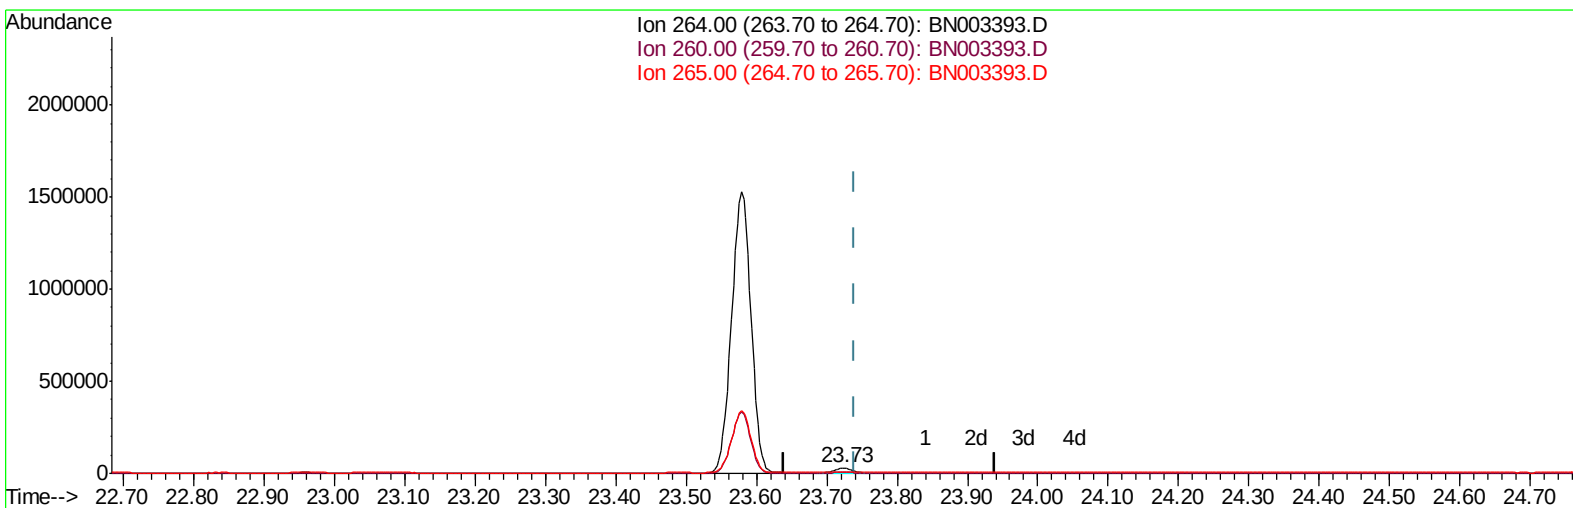

TIC: BN003393.D

(20) Perylene-d12 (I)

23.725min (-0.015) 0.40ng/ul m

response 50809

Ion	Exp%	Act%
264.00	100	100
260.00	25.60	26.17
265.00	33.70	34.40
0.00	0.00	0.00